



**SPL-LABMAT s.r.o.**  
SPL – služby pro laboratoře  
1.máje 432, 735 31 Bohumín,  
Česká republika  
tel:+420 596 014 627  
[info@spl-labmat.cz](mailto:info@spl-labmat.cz)  
[www.spl-labmat.cz](http://www.spl-labmat.cz)

Proficiency testing provider

# Report

(final)

**on the evaluation of the proficiency testing programme**

**PT 29/4A (RM SPL-L3)**

**Determination of**  
**C, Mn, Si, P, S, Cu, Cr, Ni, Al, Mo, Mg, Ce, W, V, Ti, Co, As, Sn, Zn, Zr,**  
**B, Nb**  
**in samples of ductile cast iron**  
**by atomic emission spectrometry, X-Ray fluorescence spectrometry**  
**and by validated wet-way and combustion methods**

Issued on December 1st, 2021  
Martin Bogumský, SPL-LABMAT s.r.o.

**SPL-LABMAT s.r.o.**  
1. máje 432  
735 31 Bohumín, CZ  
IČO: 06480870, DIČ: CZ06480870  
[www.spl-labmat.cz](http://www.spl-labmat.cz)  
e-mail: [info@spl-labmat.cz](mailto:info@spl-labmat.cz)



## Contents

|           |   |          |
|-----------|---|----------|
| <b>1.</b> | <b>General information on PT.....</b>                       | <b>2</b> |
| <b>2.</b> | <b>Confidentiality agreement .....</b>                      | <b>3</b> |
| <b>3.</b> | <b>Abbreviations, definitions, signs .....</b>              | <b>3</b> |
| <b>4.</b> | <b>General principles of PT.....</b>                        | <b>4</b> |
|           | <b>4.1 PT schedule .....</b>                                | <b>4</b> |
|           | <b>4.2 Conditions of participations in PT .....</b>         | <b>4</b> |
| <b>5.</b> | <b>Preparation and homogeneity of tested items .....</b>    | <b>5</b> |
| <b>6.</b> | <b>Statistic evaluation and performance standards .....</b> | <b>5</b> |
|           | <b>6.1 Reference value and related uncertainty .....</b>    | <b>5</b> |
|           | <b>6.2 Performance evaluation .....</b>                     | <b>8</b> |
| <b>7.</b> | <b>PT evaluation results summary .....</b>                  | <b>9</b> |
| <b>8.</b> | <b>Conclusion .....</b>                                     | <b>9</b> |

## 1. General information on PT (table 1)

|  |   |
|--|---|
| <b>Label</b>                                 | PT 29/4A  |
| <b>Object of PT</b>                          | Determination of C, Mn, Si, P, S, Cu, Cr, Ni, Al, Mo, Mg, Ce, W, V, Ti, Co, As, Sn, Zn, Zr, B, Nb in ductile cast iron  |
| <b>Assessment method(s)</b>                  | Atomic emission spectrometry, X-Ray fluorescence spectrometry and by validated wet-way and combustion methods   |
| <b>Item of proficiency testing:</b>          | Ductile cast iron, sample PT 29/4A  |
| <b>Date of testing</b>                       | September-October, 2021   |
| <b>Name and address of the PT provider</b>   | SPL-LABMAT s.r.o.<br>1. máje 432, 735 31 Bohumín, www.spl-labmat.cz<br>Tel: 596014627, e-mail: <a href="mailto:info@spl-labmat.cz">info@spl-labmat.cz</a>   |
| <b>Responsible person</b>                    | Ing. Martin Bogumský  |
| <b>Colaborator(s)</b>                        | Ing. Denisa Kupczynová, René Piszczek   |
| <b>Operations provided by subcontractors</b> | Providing of candidate material, preliminary chemical analysis and homogeneity analysis   |
| <b>Number of participants</b>                | 34  |
| <b>Test item description</b>                 | Sample d40x18mm, alternatively crushed sample packed in a plastic bottle (on request only).   |
| <b>Number of test items</b>                  | 40 pcs solid sample, 20 pcs crushed sample  |
| <b>Technique of sample preparation</b>       | Material was produced in induction furnace and casted in mould. Samples was prepared by machining.  |
| <b>Item and result distribution</b>          | Post and transport services, e-mail and webpages  |
| <b>Result acceptance</b>                     | Electronic in provided forms (MS Excel files)   |
| <b>Performance assessment standards</b>      | Performance assessment based on z-scoring.<br>Result z-score with $-2 \leq Z_N \leq 2$ were considered satisfactory for all elements.<br>Reference values assessed as consensual with the values provided by participants. In all cases, this was equal to the arithmetic mean of the results after outliers exclusion by Grubbs' test. Standard deviation $s_N$ for proficiency assessment was used from TPP-Fe, sp (2018) programme.  |
| <b>Homogeneity and stability</b>             | Material homogeneity was tested in the laboratory Enviform a.s. Measurements were done for three final samples, five determinations of each, 15 in total.<br>For homogeneity assessments and standard deviation calculation, the statistical method ANOVA was employed for all assessments. Material homogeneity as compared with the norms for assessment of elements in steel/cast iron proved satisfactory for the PT. Homogeneity assessments were done for all elements. Given the character of the tested items, any influences of time and environment instability are excluded. |

## 2. Confidentiality agreement

The provider of PT declares that all information and data pertinent to the individual participants are considered confidential and dealt with accordingly. Participant code numbers are assigned at random for each participant and each PT independently. In the final report, results are identified by code numbers only and are therefore anonymous.

## 3. Abbreviations, definitions and signs

|          |                                 |
|----------|---------------------------------|
| PT       | proficiency testing             |
| PT XX/XX | item labelling (samples) for PT |

### Participant in PT

laboratory, company or private person who receives the items for PT and submits the results to the PT provider

### Accepted laboratory result

laboratory result which has not been excluded as outlying

|              |   |
|--------------|---|
| $x$          | laboratory result representing the arithmetic mean of (usually) five results submitted by participants                      |
| $s$          | selected standard deviation for five laboratory assessments for a given element   |
| $t_{5;0,05}$ | confidence level for five assessments for the reliability level 95%   |
| $u$          | repeatability of five results for one participant, $u = \pm \frac{t_{5;0,05}}{\sqrt{5}} \cdot s$                            |
| $n$          | number of participants involved in the statistical data set after exclusion of outliers                                     |
| $X$          | reference value, see 6.1 for details on assessment  |
| $X_{Ref}$    | reference value calculated as mean of the values of selected participating laboratories                                     |
| $X_{PT}$     | consensual estimate of the mean value of laboratory results performed according to a method suitable for their distribution |
| $s_{PT}$     | selected standard deviation from the statistical data set in PT   |
| $s_N$        | selected standard deviation as listed in the norm for determination of the given element                                    |
| $Z_{PT}$     | z-score derived from $s_{PT}$ , see chapter 6.2   |

|       |   |
|-------|---|
| $Z_N$ | z-score derived from $s_N$ , see chapter 6.2  |
| $U$   | Uncertainty of the reference value, extended uncertainty (extension factor=2) in the sense of the ISO Guide to the Expression of the Uncertainty of Measurement (1993), dependent on the standard deviation of the laboratory results. This is expressed as a one half of a $\pm$ interval. |

## 4. General principles of the PT

PT was organized, executed and evaluated according to the ČSN EN ISO/IEC 17043:2010.

### 4.1 PT schedule

Information about the PT were made public on the web site of the provider. Those laboratories that had previously expressed interest in receiving information on the next PT were informed by email. Instructions for participants were part of the PT programme and were also distributed along with the test item. The sample remains property of the participant once the PT has been concluded.

### 4.2 Conditions for PT participation

By agreeing to participate in the PT, the participants committed to deliver within the designated period five parallel results of analyses, performed under the repeatability conditions (i.e. performed with the exact same equipment in an immediate and uninterrupted sequence). According to the requirements of the norm ČSN EN ISO/IEC 17043:2010 every measurement for the PT should be performed as a routine measurement that is under the same conditions and procedures as are usual in the everyday operation of the laboratory. The assessment method and (alternatively) the category and type of equipment are given by the participant in the PT protocol which was publicly accessible during the PT period at the web site of the provider [www.spl-labmat.cz](http://www.spl-labmat.cz).

Based on the experience of the previous years, all the results submitted by participants, regardless of the method and equipment used, were included in the statistical data set. For evaluation, outlier exclusion was employed or alternatively robust statistics for elimination of the influence of outliers on the reference value and corresponding uncertainty.

**Once the PT has been completed, the participants are provided:**

**Final report** on the evaluation incl. evaluation of individual analytes.

**Certificate** of participation on the PT including two annexes.

**Certificate of chemical analysis** for new reference material

## 5. Preparation and homogeneity of the test items

Details concerning the preparation of the test items and measurements of homogeneity for this PT are presented in the **table 1 – general information on the PT**.

For the evaluation of homogeneity, we have employed our own programme using the statistical method ANOVA along with calculation of the standard deviation  $s$  from all assessments and their

comparison to the usual values according to the norms or previous PTs. As the criterion of sufficient homogeneity for the purpose of the PT, the condition to be met is  $s < 0,5 s_N$ , where  $s$  is the standard deviation in the measurement of homogeneity and  $s_N$  is the standard deviation according to the norm. Where no valid norm is available, an older norm with expired validity or a norm used in another country can be consulted, or comparison with values from previous PTs for similar materials. In case the  $s < 0,5 s_N$  criterion is not met for some of the assessed parameters, non-homogeneity contribution can be taken into account by increasing  $s_{PT}$  and  $s_N$  for  $z$ -scoring assessment, in the following manner:

$$s_{PT}^* = \sqrt{s_{PT}^2 + s^2}$$

$$s_N^* = \sqrt{s_N^2 + s^2}$$

## 6. Statistic evaluation and performance standards

### 6.1 Reference value and related uncertainty

The statistical methods employed were used according to the norms ISO 13528:2005, ČSN ISO 5725-2:1997 a ČSN ISO 2602:1993.

Mean value of five results submitted by a single contributor is the **laboratory mean  $x$** , which is equivalent to the arithmetic mean from five measurements and which represents the result of the laboratory for individual elements. The value of the measurement **uncertainty  $u$**  (repeatability), calculated from five assessments of a single laboratory, is also given.

This laboratory mean is given in bold on the pages with evaluation results for individual elements and it is used for subsequent statistical evaluation of laboratory results – that is statistical data sets for individual elements. Uncertainty  $u$  is given in the column on the right along with the laboratory mean  $x$ .

On the basis of this data set, the reference value is assessed and also the corresponding uncertainty. Also, if need be, Grubbs test according to the ČSN ISO 5725-2 is used to eliminate outlying results. Given the usual character of results in the provider's PT, in great majority of cases **consensual estimate of the reference value  $X_{PT}$**  is used. This can be calculated according to several statistical methods according to the algorithm given below. In this case the reference value on the page is marked  $\hat{X} = X_{PT}$ .

Where the provider considers it appropriate, in unique cases the reference value can be established on the basis of the results from selected laboratories with a long history of reliable results, where the probability of correct determination is higher. In these cases reference value in the table is marked as  $\hat{X} = X_{Ref}$ .

**Basic statistical terms used**


|  |   |
|--|---|
| $n$  | number of laboratories  |
| $p_i$  | number of assessments in $i$ -th laboratory   |
| $y_{ik}$   | result of $k$ -th assessment in the $i$ -th laboratory                                |
| $i \in \{1, \dots, n\}$  | laboratory index  |
| $k \in \{1, \dots, p_i\}$  | assessment index in the $i$ -th laboratory  |
| $x_i = \bar{y} = \frac{1}{n_i} \sum_{k=1}^{p_i} y_{ik}$                | mean value of assessment in th $i$ -th laboratory                                     |
| $\bar{y} = \bar{x} = \frac{1}{n} \sum_{i=1}^n x_i$                     | mean value of evaluation from all laboratories  |
| $s_i^2 = \frac{1}{p_i-1} \sum_{k=1}^{p_i} (y_{ik} - \bar{y}_i)^2$      | variance in $i$ -th laboratory  |
| $s_{PT}^2 = \frac{1}{n-1} \sum_{i=1}^n (x_i - \bar{x})^2$              | value variance from all laboratories  |
| $s_i = \sqrt{\frac{1}{p_i-1} \sum_{k=1}^{p_i} (y_{ik} - \bar{y}_i)^2}$ | selected standard deviation of individual laboratory results                          |
| $s_{PT} = \sqrt{\frac{1}{p-1} \sum_{i=1}^p (x_i - \bar{x})^2}$         | selected standard deviation of the data set from all participating laboratories in PT |
| $u_i = \pm \frac{t_{5;0,05}}{\sqrt{5}} \cdot s_i$                      | determination uncertainty (repeatability)   |
| $U = \pm \frac{t_{5;0,05}}{\sqrt{n}} \cdot s_{PT}$                     | reference value uncertainty   |

**Reference to the statistical methods used for the assessment of the reference value and its uncertainty**

- **Arithmetic mean for elimination of outlying values by the Grubbs' test** according to ČSN ISO 5725-2.
- Robust method analysis based on median regression **MAD** (Montfort, M.A.J.von, Commun. Soil. Sci. Plant. Anal. 27, 463-468 (1996). This method is employed whenever the difference between AVG a MAD is above  $0,5s_{PT}$  and at the same time, the number of laboratory means submitted is above 15.
- **Horn's procedures** (J. Horn, J. Am. Stat. Assoc., Volume 78, Page 930 (1983). Consensual reference value, robust method suitable for a smaller number of accepted laboratory means. It is being employed under the same conditions as the MAD, only for a lower number of accepted laboratory means, between 8 and 14. Whenever the number of laboratories is equal to or below 7 reference value is not assessed, or alternatively only as an informative value.



**Evaluation algorithm:**

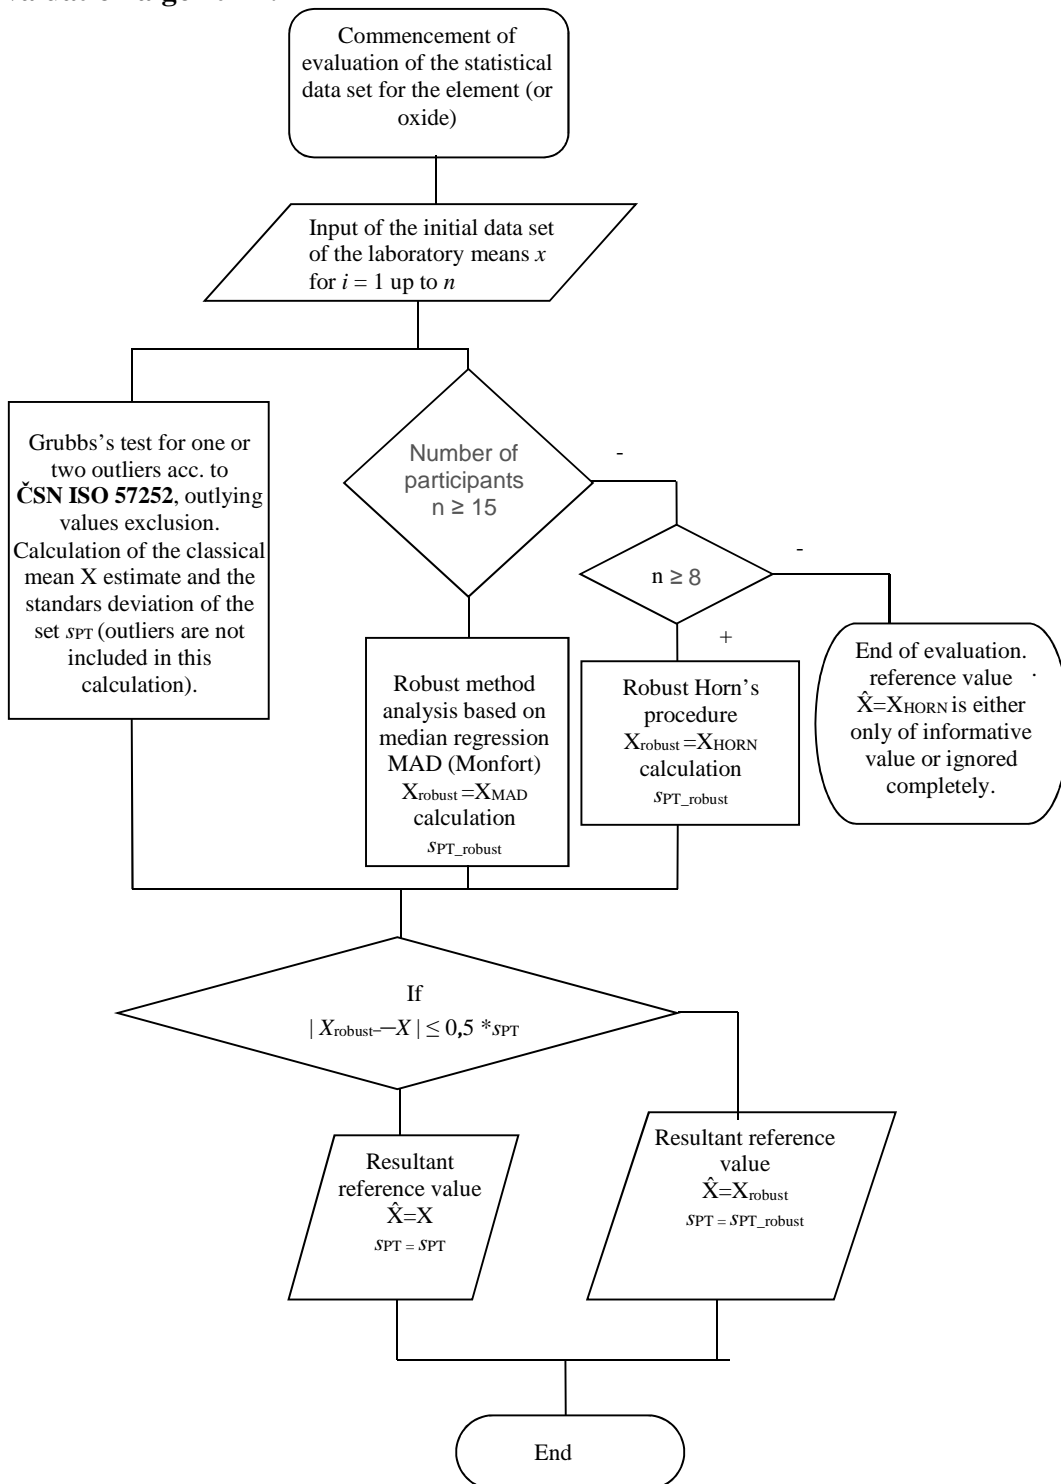

## 6.2 Performance evaluation

z-scoring is done both for **subjective**  $Z_{PT}$ , i.e. calculated from the participants' data set – deviation  $s_{PT}$

$$Z_{PT} = \frac{x - X}{s_{PT}}$$

and **objective**  $Z_N$ , based on the deviation given above derived from the norm  $s_N$  (if available), where

$$Z_N = \frac{x - X}{s_N}$$

If the  $s_N$  deviation is not available, subjective z-scoring  $Z_{PT}$  is used to assess the performance of the laboratory.

**If the  $s_N$  deviation is available, the objective z-scoring  $Z_N$  is used to evaluate the performance and the subjective z-score  $Z_{PT}$  has only informative value.** In a very limited number of cases, where the variability of laboratory means was larger, the subjective z-scoring was applied as criterion for individual elements.

Performance value of  $|Z_N| \leq 2$  is considered „**satisfactory**“

Performance value of  $2 < |Z_N| \leq 3$  is considered „**problematic**“

Performance value of  $|Z_N| > 3$  is considered „**unsuitable**“.

**Problematic** performance value calls for attention, **unsuitable** performance calls for correction.

## 7. PT evaluation results summary

Table 2

| Element | $X$<br>[%wt.] | $U$<br>[%wt.] | $s_{PT}$<br>[%wt.] | $s_N$<br>[%wt.] | No of<br>laboratories<br>in the data<br>set | Overall No<br>of<br>laboratories | No of<br>laboratories<br>where the<br>criteria<br>were<br>exceeded |
|---------|---------------|---------------|--------------------|-----------------|---|----------------------------------|--|
| C       | <b>3.533</b>  | 0.022         | 0.055              | 0.073           | 27  | 27                               | 0  |
| Mn      | <b>1.414</b>  | 0.012         | 0.031              | 0.025           | 30  | 30                               | 4  |
| Si      | <b>3.006</b>  | 0.029         | 0.076              | 0.066           | 29  | 29                               | 2  |
| P       | <b>0.074</b>  | 0.002         | 0.005              | 0.006           | 28  | 28                               | 0  |
| S       | <b>0.0106</b> | 0.0005        | 0.0013             | 0.0016          | 28  | 29                               | 1  |
| Cu      | <b>0.690</b>  | 0.006         | 0.016              | 0.016           | 29  | 29                               | 2  |
| Cr      | <b>0.669</b>  | 0.007         | 0.018              | 0.017           | 30  | 30                               | 1  |
| Ni      | <b>1.027</b>  | 0.007         | 0.019              | 0.022           | 30  | 30                               | 0  |
| Al      | <b>0.0240</b> | 0.0010        | 0.0021             | 0.0026          | 20  | 21                               | 1  |
| Mo      | <b>0.055</b>  | 0.002         | 0.004              | 0.004           | 29  | 29                               | 0  |
| Mg      | <b>0.048</b>  | 0.002         | 0.004              | 0.005           | 23  | 23                               | 0  |
| Ce      | <b>0.034</b>  | 0.002         | 0.003              | 0.006           | 13  | 13                               | 0  |
| W       | <b>0.0141</b> | 0.0017        | 0.0029             | 0.0037          | 14  | 14                               | 0  |
| V       | <b>0.351</b>  | 0.004         | 0.008              | 0.010           | 22  | 23                               | 1  |
| Ti      | <b>0.080</b>  | 0.003         | 0.006              | 0.007           | 24  | 24                               | 0  |
| Co      | <b>0.059</b>  | 0.001         | 0.003              | 0.004           | 21  | 21                               | 0  |
| As      | <b>0.0078</b> | 0.0007        | 0.0012             | 0.0021          | 13  | 13                               | 0  |
| Sn      | <b>0.0234</b> | 0.0007        | 0.0014             | 0.0027          | 20  | 21                               | 1  |
| Zn      | <b>0.0194</b> | 0.0011        | 0.0023             | 0.0028          | 18  | 18                               | 0  |
| Zr      | <b>0.042</b>  | 0.002         | 0.002              | 0.002           | 9   | 9                                | 0  |
| B       | <b>0.0036</b> | 0.0002        | 0.0003             | 0.0005          | 12  | 12                               | 0  |
| Nb      | <b>0.0099</b> | 0.0007        | 0.0013             | 0.0018          | 16  | 17                               | 1  |

$X$  – reference value

$U$  – reference value uncertainty

$s_{PT}$  – data set standard deviation

$s_N$  – standard deviation according to the norm

## 8. Conclusion

The result dispersion is fully comparable to the previous rounds of PT for cast iron chem. composition determination. Names of participating laboratories are stated in the Certificate of chemical analysis. Reference material produced as the result of PT 29/4A is named **SPL-L3**.


# PT 29/4A - C

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 1           |                  | -   |       |       |       |       |              |               |                       |                      |
| 18          |                  | -   |       |       |       |       |              |               |                       |                      |
| 21          |                  | -   |       |       |       |       |              |               |                       |                      |
| 23          |                  | -   |       |       |       |       |              |               |                       |                      |
| 27          |                  | -   |       |       |       |       |              |               |                       |                      |
| 29          |                  | -   |       |       |       |       |              |               |                       |                      |
| 33          |                  | -   |       |       |       |       |              |               |                       |                      |
| 10          | AES              | 3,450   | 3,440 | 3,450 | 3,440 | 3,460 | <b>3,448</b> | 0,010         | -1,55                 | -1,16                |
| 12          | AES              | 3,440   | 3,450 | 3,470 | 3,470 | 3,470 | <b>3,460</b> | 0,018         | -1,33                 | -1,00                |
| 11          | AES              | 3,450   | 3,450 | 3,450 | 3,490 | 3,470 | <b>3,462</b> | 0,022         | -1,29                 | -0,97                |
| 28          | IR               | 3,489   | 3,498 | 3,435 | 3,482 | 3,455 | <b>3,472</b> | 0,032         | -1,11                 | -0,84                |
| 8           | AES              | 3,470   | 3,460 | 3,480 | 3,480 | 3,470 | <b>3,472</b> | 0,010         | -1,11                 | -0,84                |
| 9           | AES              | 3,450   | 3,480 | 3,480 | 3,500 | 3,470 | <b>3,476</b> | 0,023         | -1,04                 | -0,78                |
| 13          | AES              | 3,480   | 3,500 | 3,480 | 3,490 | 3,520 | <b>3,494</b> | 0,021         | -0,71                 | -0,53                |
| 16          | IR               | 3,504   | 3,502 | 3,489 | 3,484 | 3,503 | <b>3,496</b> | 0,011         | -0,67                 | -0,51                |
| 17          | IR               | 3,490   | 3,510 | 3,500 | 3,485 | 3,495 | <b>3,496</b> | 0,012         | -0,67                 | -0,51                |
| 20          | AES              | 3,498   | 3,487 | 3,525 | 3,496 | 3,507 | <b>3,503</b> | 0,018         | -0,55                 | -0,41                |
| 3           | AES              | 3,514   | 3,515 | 3,505 | 3,516 | 3,522 | <b>3,514</b> | 0,008         | -0,35                 | -0,26                |
| 7           | IR               | 3,516   | 3,508 | 3,503 | 3,514 | 3,546 | <b>3,517</b> | 0,021         | -0,29                 | -0,22                |
| 15          | IR               | 3,518   | 3,511 | 3,531 | 3,518 | 3,517 | <b>3,519</b> | 0,009         | -0,25                 | -0,19                |
| 34          | IR               | 3,533   | 3,520 | 3,528 | 3,530 | 3,537 | <b>3,530</b> | 0,008         | -0,05                 | -0,04                |
| 32          | AES              | 3,514   | 3,543 | 3,548 | 3,527 | 3,522 | <b>3,531</b> | 0,018         | -0,04                 | -0,03                |
| 14          | AES              | 3,546   | 3,527 | 3,530 | 3,529 | 3,538 | <b>3,534</b> | 0,010         | 0,02                  | 0,01                 |
| 31          | AES              | 3,546   | 3,527 | 3,534 | 3,529 | 3,538 | <b>3,535</b> | 0,009         | 0,04                  | 0,03                 |
| 2           | XRF              | 3,661   | 3,609 | 3,599 | 3,312 | 3,621 | <b>3,560</b> | 0,175         | 0,49                  | 0,37                 |
| 22          | IR               | 3,570   | 3,582 | 3,542 | 3,565 | 3,559 | <b>3,564</b> | 0,018         | 0,56                  | 0,42                 |
| 5           | AES              | 3,566   | 3,572 | 3,561 | 3,560 | 3,560 | <b>3,564</b> | 0,006         | 0,56                  | 0,42                 |
| 4           | IR               | 3,570   | 3,572 |       |       |       | <b>3,571</b> |               | 0,69                  | 0,52                 |
| 6           | AES              | 3,636   | 3,572 | 3,556 | 3,577 | 3,608 | <b>3,590</b> | 0,040         | 1,04                  | 0,78                 |
| 24          | AES              | 3,605   | 3,602 | 3,600 | 3,605 | 3,605 | <b>3,603</b> | 0,003         | 1,27                  | 0,96                 |
| 25          | AES              | 3,600   | 3,601 | 3,605 | 3,603 | 3,605 | <b>3,603</b> | 0,003         | 1,27                  | 0,96                 |
| 30          | IR               | 3,590   | 3,610 | 3,590 | 3,630 | 3,620 | <b>3,608</b> | 0,022         | 1,36                  | 1,03                 |
| 19          | AES              | 3,620   | 3,570 | 3,590 | 3,650 | 3,650 | <b>3,616</b> | 0,044         | 1,51                  | 1,14                 |
| 26          | AES              | 3,662   | 3,660 | 3,650 | 3,660 | 3,661 | <b>3,659</b> | 0,006         | 2,29                  | 1,73                 |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 27 | 3,533                     | 0,055                  | 0,073                 | 0,022    |

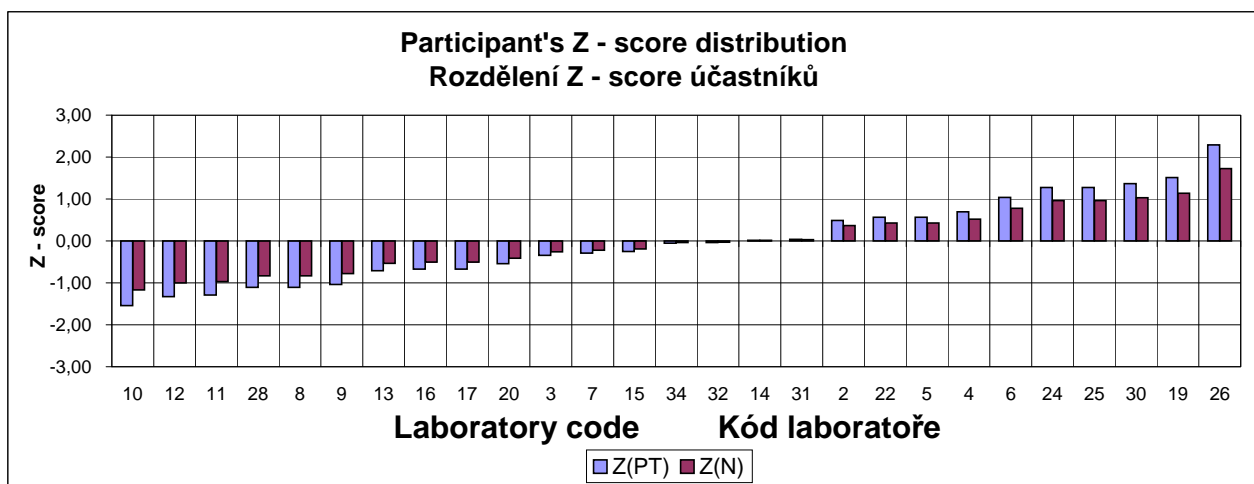


# PT 29/4A - Mn

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 23          | ICP              | 1,337   | 1,350 | 1,345 | 1,345 | 1,340 | <b>1,343</b>     | 0,006                  | -2,29                                    | -2,84                                  |
| 21          | Photometric      | 1,346   | 1,367 | 1,359 | 1,353 | 1,362 | <b>1,357</b>     | 0,010                  | -1,84                                    | -2,28                                  |
| 7           | AES              | 1,362   | 1,371 | 1,366 | 1,369 | 1,366 | <b>1,367</b>     | 0,004                  | -1,52                                    | -1,88                                  |
| 6           | AES              | 1,374   | 1,367 | 1,362 | 1,394 | 1,367 | <b>1,373</b>     | 0,016                  | -1,32                                    | -1,64                                  |
| 27          | XRF              | 1,382   | 1,375 | 1,384 | 1,379 | 1,382 | <b>1,380</b>     | 0,004                  | -1,10                                    | -1,36                                  |
| 33          | XRF              | 1,383   | 1,380 | 1,377 | 1,379 | 1,384 | <b>1,381</b>     | 0,004                  | -1,06                                    | -1,32                                  |
| 2           | XRF              | 1,399   | 1,393 | 1,396 | 1,396 | 1,397 | <b>1,396</b>     | 0,003                  | -0,58                                    | -0,72                                  |
| 14          | AES              | 1,394   | 1,409 | 1,393 | 1,391 | 1,401 | <b>1,398</b>     | 0,009                  | -0,52                                    | -0,64                                  |
| 30          | AES              | 1,390   | 1,400 | 1,400 | 1,400 | 1,400 | <b>1,398</b>     | 0,006                  | -0,52                                    | -0,64                                  |
| 32          | AES              | 1,411   | 1,403 | 1,398 | 1,391 | 1,390 | <b>1,399</b>     | 0,011                  | -0,48                                    | -0,60                                  |
| 28          | ICP              | 1,395   | 1,398 | 1,405 | 1,395 | 1,408 | <b>1,400</b>     | 0,007                  | -0,45                                    | -0,56                                  |
| 20          | AES              | 1,413   | 1,402 | 1,413 | 1,405 | 1,408 | <b>1,408</b>     | 0,006                  | -0,19                                    | -0,24                                  |
| 5           | AES              | 1,413   | 1,406 | 1,407 | 1,415 | 1,415 | <b>1,411</b>     | 0,005                  | -0,10                                    | -0,12                                  |
| 17          | ICP              | 1,428   | 1,395 | 1,409 | 1,412 | 1,447 | <b>1,418</b>     | 0,025                  | 0,13                                     | 0,16                                   |
| 31          | AES              | 1,422   | 1,421 | 1,424 | 1,419 | 1,407 | <b>1,419</b>     | 0,008                  | 0,16                                     | 0,20                                   |
| 4           | AES              | 1,440   | 1,400 | 1,420 |       |       | <b>1,420</b>     | 0,050                  | 0,19                                     | 0,24                                   |
| 3           | AES              | 1,423   | 1,418 | 1,423 | 1,428 | 1,420 | <b>1,422</b>     | 0,005                  | 0,26                                     | 0,32                                   |
| 12          | AES              | 1,430   | 1,427 | 1,430 | 1,424 | 1,429 | <b>1,428</b>     | 0,003                  | 0,45                                     | 0,56                                   |
| 11          | AES              | 1,432   | 1,432 | 1,431 | 1,430 | 1,427 | <b>1,430</b>     | 0,003                  | 0,52                                     | 0,64                                   |
| 13          | AES              | 1,431   | 1,432 | 1,429 | 1,430 | 1,429 | <b>1,430</b>     | 0,002                  | 0,52                                     | 0,64                                   |
| 9           | AES              | 1,431   | 1,431 | 1,431 | 1,431 | 1,433 | <b>1,431</b>     | 0,001                  | 0,55                                     | 0,68                                   |
| 10          | AES              | 1,430   | 1,438 | 1,428 | 1,433 | 1,429 | <b>1,432</b>     | 0,005                  | 0,58                                     | 0,72                                   |
| 8           | AES              | 1,434   | 1,434 | 1,435 | 1,436 | 1,434 | <b>1,435</b>     | 0,001                  | 0,68                                     | 0,84                                   |
| 18          | AES              | 1,424   | 1,437 | 1,434 | 1,444 | 1,437 | <b>1,435</b>     | 0,009                  | 0,68                                     | 0,84                                   |
| 19          | AES              | 1,430   | 1,430 | 1,440 | 1,440 | 1,440 | <b>1,436</b>     | 0,007                  | 0,71                                     | 0,88                                   |
| 1           | AES              | 1,429   | 1,439 | 1,444 | 1,432 | 1,436 | <b>1,436</b>     | 0,007                  | 0,71                                     | 0,88                                   |
| 29          | AES              | 1,442   | 1,439 | 1,449 | 1,440 | 1,449 | <b>1,444</b>     | 0,006                  | 0,97                                     | 1,20                                   |
| 24          | AES              | 1,458   | 1,456 | 1,456 | 1,453 | 1,458 | <b>1,456</b>     | 0,003                  | 1,35                                     | 1,68                                   |
| 26          | AES              | 1,466   | 1,465 | 1,465 | 1,466 | 1,462 | <b>1,465</b>     | 0,002                  | 1,65                                     | 2,04                                   |
| 25          | AES              | 1,475   | 1,470 | 1,472 | 1,470 | 1,475 | <b>1,472</b>     | 0,003                  | 1,87                                     | 2,32                                   |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 30 | 1,414                     | 0,031                  | 0,025                 | 0,012    |

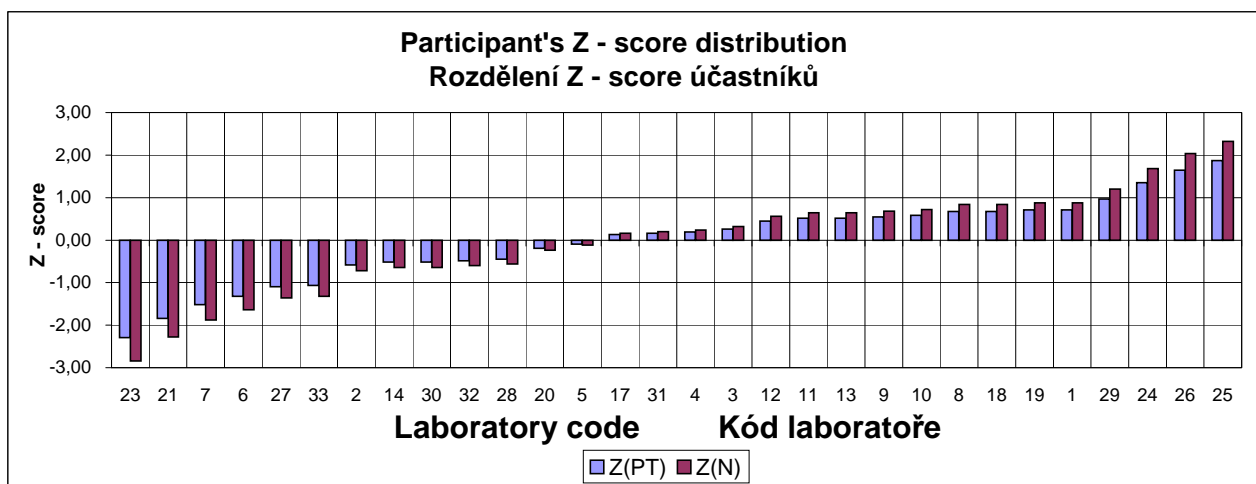


# PT 29/4A - Si

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 15          |                  | -   |       |       |       |       |              |               |                       |                      |
| 16          |                  | -   |       |       |       |       |              |               |                       |                      |
| 22          |                  | -   |       |       |       |       |              |               |                       |                      |
| 28          |                  | -   |       |       |       |       |              |               |                       |                      |
| 34          |                  | -   |       |       |       |       |              |               |                       |                      |
| 21          | Photometric      | 2,881   | 2,822 | 2,835 | 2,832 | 2,863 | <b>2,847</b> | 0,030         | -2,09                 | -2,41                |
| 6           | AES              | 2,917   | 2,876 | 2,889 | 2,846 | 2,843 | <b>2,874</b> | 0,038         | -1,74                 | -2,00                |
| 4           | AES              | 2,850   | 2,930 | 2,870 |       |       | <b>2,883</b> | 0,103         | -1,62                 | -1,86                |
| 18          | AES              | 2,886   | 2,914 | 2,893 | 2,928 | 2,875 | <b>2,899</b> | 0,027         | -1,41                 | -1,62                |
| 2           | XRF              | 2,892   | 3,011 | 2,912 | 2,938 | 2,989 | <b>2,948</b> | 0,063         | -0,76                 | -0,88                |
| 17          | Gravimetric      | 2,960   | 2,976 | 2,956 | 2,933 | 2,944 | <b>2,954</b> | 0,020         | -0,68                 | -0,79                |
| 3           | AES              | 2,959   | 2,948 | 2,952 | 2,954 | 2,959 | <b>2,954</b> | 0,006         | -0,68                 | -0,79                |
| 5           | AES              | 2,998   | 2,946 | 2,986 | 2,971 | 2,958 | <b>2,972</b> | 0,026         | -0,45                 | -0,52                |
| 20          | AES              | 2,972   | 2,994 | 2,981 | 2,980 | 2,967 | <b>2,979</b> | 0,013         | -0,36                 | -0,41                |
| 10          | AES              | 2,997   | 2,987 | 2,955 | 2,944 | 3,016 | <b>2,980</b> | 0,037         | -0,34                 | -0,39                |
| 33          | XRF              | 2,990   | 3,007 | 2,981 | 2,979 | 2,977 | <b>2,987</b> | 0,015         | -0,25                 | -0,29                |
| 8           | AES              | 3,017   | 2,999 | 2,988 | 2,954 | 2,984 | <b>2,988</b> | 0,029         | -0,24                 | -0,27                |
| 12          | AES              | 2,976   | 2,941 | 2,970 | 3,016 | 3,058 | <b>2,992</b> | 0,056         | -0,18                 | -0,21                |
| 14          | AES              | 2,979   | 2,999 | 3,029 | 3,022 | 2,974 | <b>3,001</b> | 0,031         | -0,07                 | -0,08                |
| 11          | AES              | 3,006   | 3,001 | 2,995 | 3,022 | 2,996 | <b>3,004</b> | 0,014         | -0,03                 | -0,03                |
| 9           | AES              | 3,019   | 3,004 | 3,007 | 3,020 | 3,001 | <b>3,010</b> | 0,011         | 0,05                  | 0,06                 |
| 32          | AES              | 3,022   | 3,011 | 3,034 | 3,002 | 3,029 | <b>3,020</b> | 0,016         | 0,18                  | 0,21                 |
| 19          | AES              | 3,030   | 3,020 | 3,000 | 3,030 | 3,030 | <b>3,022</b> | 0,016         | 0,21                  | 0,24                 |
| 13          | AES              | 3,041   | 3,020 | 3,042 | 3,004 | 3,009 | <b>3,023</b> | 0,022         | 0,22                  | 0,26                 |
| 29          | AES              | 3,036   | 3,043 | 3,045 | 3,041 | 3,032 | <b>3,039</b> | 0,007         | 0,43                  | 0,50                 |
| 1           | AES              | 3,046   | 3,044 | 3,036 | 3,078 | 3,070 | <b>3,055</b> | 0,023         | 0,64                  | 0,74                 |
| 27          | XRF              | 3,068   | 3,071 | 3,051 | 3,058 | 3,050 | <b>3,060</b> | 0,012         | 0,71                  | 0,82                 |
| 30          | AES              | 3,050   | 3,080 | 3,100 | 3,060 | 3,020 | <b>3,062</b> | 0,038         | 0,74                  | 0,85                 |
| 7           | AES              | 3,094   | 3,083 | 3,096 | 3,022 | 3,092 | <b>3,077</b> | 0,039         | 0,93                  | 1,08                 |
| 31          | AES              | 3,070   | 3,082 | 3,085 | 3,076 | 3,080 | <b>3,079</b> | 0,007         | 0,96                  | 1,11                 |
| 23          | ICP              | 3,089   | 3,090 | 3,090 | 3,089 | 3,086 | <b>3,089</b> | 0,002         | 1,09                  | 1,26                 |
| 26          | AES              | 3,100   | 3,091 | 3,095 | 3,100 | 3,098 | <b>3,097</b> | 0,005         | 1,20                  | 1,38                 |
| 25          | AES              | 3,090   | 3,100 | 3,110 | 3,098 | 3,100 | <b>3,100</b> | 0,009         | 1,24                  | 1,42                 |
| 24          | AES              | 3,190   | 3,192 | 3,192 | 3,189 | 3,192 | <b>3,191</b> | 0,002         | 2,43                  | 2,80                 |

| n  | $\hat{X} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 29 | 3,006                     | 0,076                  | 0,066                 | 0,029    |

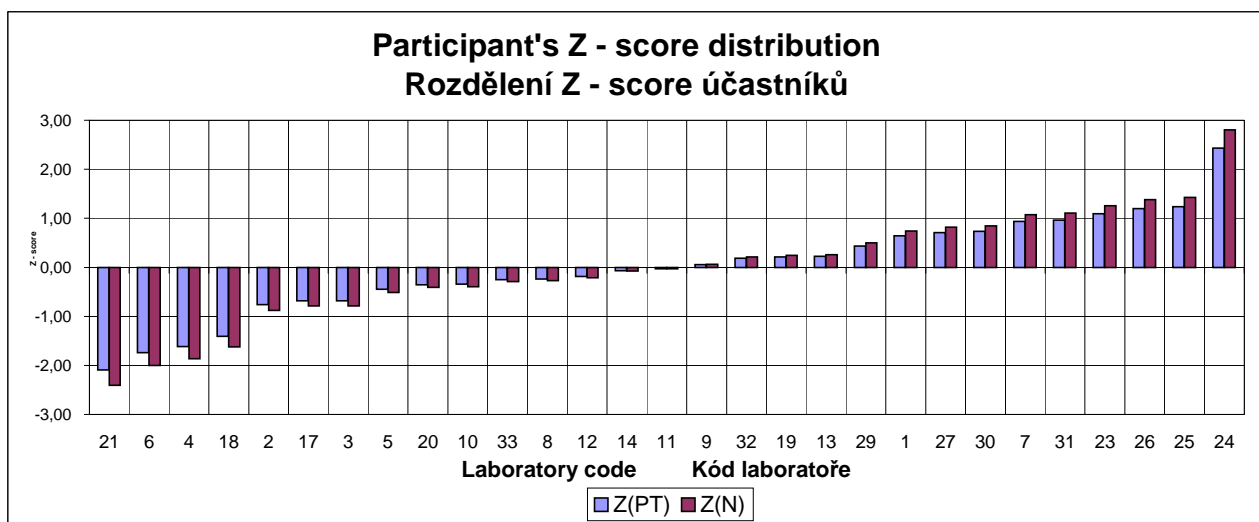


# PT 29/4A - P

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 15          |                  | -   |       |       |       |       |              |               |                       |                      |
| 16          |                  | -   |       |       |       |       |              |               |                       |                      |
| 17          |                  | -   |       |       |       |       |              |               |                       |                      |
| 22          |                  | -   |       |       |       |       |              |               |                       |                      |
| 29          |                  | -   |       |       |       |       |              |               |                       |                      |
| 34          |                  | -   |       |       |       |       |              |               |                       |                      |
| 21          | Photometric      | 0,064   | 0,066 | 0,065 | 0,064 | 0,064 | <b>0,064</b> | 0,001         | -2,00                 | -1,67                |
| 2           | XRF              | 0,064   | 0,065 | 0,063 | 0,064 | 0,063 | <b>0,064</b> | 0,001         | -2,00                 | -1,67                |
| 23          | ICP              | 0,068   | 0,069 | 0,069 | 0,068 | 0,068 | <b>0,068</b> | 0,001         | -1,20                 | -1,00                |
| 27          | XRF              | 0,068   | 0,068 | 0,069 | 0,068 | 0,066 | <b>0,068</b> | 0,001         | -1,20                 | -1,00                |
| 32          | AES              | 0,069   | 0,068 | 0,069 | 0,069 | 0,069 | <b>0,069</b> | 0,001         | -1,00                 | -0,83                |
| 33          | XRF              | 0,069   | 0,069 | 0,069 | 0,069 | 0,069 | <b>0,069</b> | 0,000         | -1,00                 | -0,83                |
| 19          | AES              | 0,069   | 0,071 | 0,072 | 0,067 | 0,065 | <b>0,069</b> | 0,004         | -1,00                 | -0,83                |
| 5           | AES              | 0,069   | 0,067 | 0,074 | 0,071 | 0,069 | <b>0,070</b> | 0,003         | -0,80                 | -0,67                |
| 4           | AES              | 0,074   | 0,068 | 0,071 |       |       | <b>0,071</b> | 0,007         | -0,60                 | -0,50                |
| 3           | AES              | 0,072   | 0,069 | 0,071 | 0,071 | 0,072 | <b>0,071</b> | 0,002         | -0,60                 | -0,50                |
| 24          | AES              | 0,072   | 0,071 | 0,071 | 0,072 | 0,071 | <b>0,071</b> | 0,001         | -0,60                 | -0,50                |
| 26          | AES              | 0,071   | 0,072 | 0,071 | 0,073 | 0,070 | <b>0,071</b> | 0,001         | -0,60                 | -0,50                |
| 25          | AES              | 0,070   | 0,073 | 0,071 | 0,072 | 0,071 | <b>0,071</b> | 0,001         | -0,60                 | -0,50                |
| 6           | AES              | 0,070   | 0,073 | 0,077 | 0,071 | 0,071 | <b>0,072</b> | 0,003         | -0,40                 | -0,33                |
| 20          | AES              | 0,073   | 0,073 | 0,073 | 0,074 | 0,073 | <b>0,073</b> | 0,001         | -0,20                 | -0,17                |
| 18          | AES              | 0,071   | 0,074 | 0,074 | 0,074 | 0,074 | <b>0,073</b> | 0,002         | -0,20                 | -0,17                |
| 1           | AES              | 0,073   | 0,073 | 0,073 | 0,074 | 0,075 | <b>0,074</b> | 0,001         | 0,00                  | 0,00                 |
| 30          | AES              | 0,075   | 0,073 | 0,076 | 0,076 | 0,074 | <b>0,075</b> | 0,002         | 0,20                  | 0,17                 |
| 14          | AES              | 0,080   | 0,076 | 0,075 | 0,075 | 0,077 | <b>0,077</b> | 0,003         | 0,60                  | 0,50                 |
| 28          | ICP              | 0,079   | 0,077 | 0,077 | 0,077 | 0,076 | <b>0,077</b> | 0,002         | 0,60                  | 0,50                 |
| 7           | AES              | 0,079   | 0,078 | 0,080 | 0,076 | 0,078 | <b>0,078</b> | 0,002         | 0,80                  | 0,67                 |
| 11          | AES              | 0,081   | 0,080 | 0,079 | 0,081 | 0,080 | <b>0,080</b> | 0,001         | 1,20                  | 1,00                 |
| 8           | AES              | 0,080   | 0,080 | 0,080 | 0,082 | 0,080 | <b>0,080</b> | 0,001         | 1,20                  | 1,00                 |
| 10          | AES              | 0,079   | 0,080 | 0,081 | 0,081 | 0,081 | <b>0,080</b> | 0,001         | 1,20                  | 1,00                 |
| 31          | AES              | 0,077   | 0,075 | 0,088 | 0,074 | 0,084 | <b>0,080</b> | 0,008         | 1,20                  | 1,00                 |
| 9           | AES              | 0,080   | 0,081 | 0,080 | 0,083 | 0,079 | <b>0,081</b> | 0,002         | 1,40                  | 1,17                 |
| 12          | AES              | 0,080   | 0,081 | 0,079 | 0,082 | 0,081 | <b>0,081</b> | 0,001         | 1,40                  | 1,17                 |
| 13          | AES              | 0,081   | 0,081 | 0,083 | 0,080 | 0,084 | <b>0,082</b> | 0,002         | 1,60                  | 1,33                 |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 28 | 0,074                     | 0,005                  | 0,006                 | 0,002    |

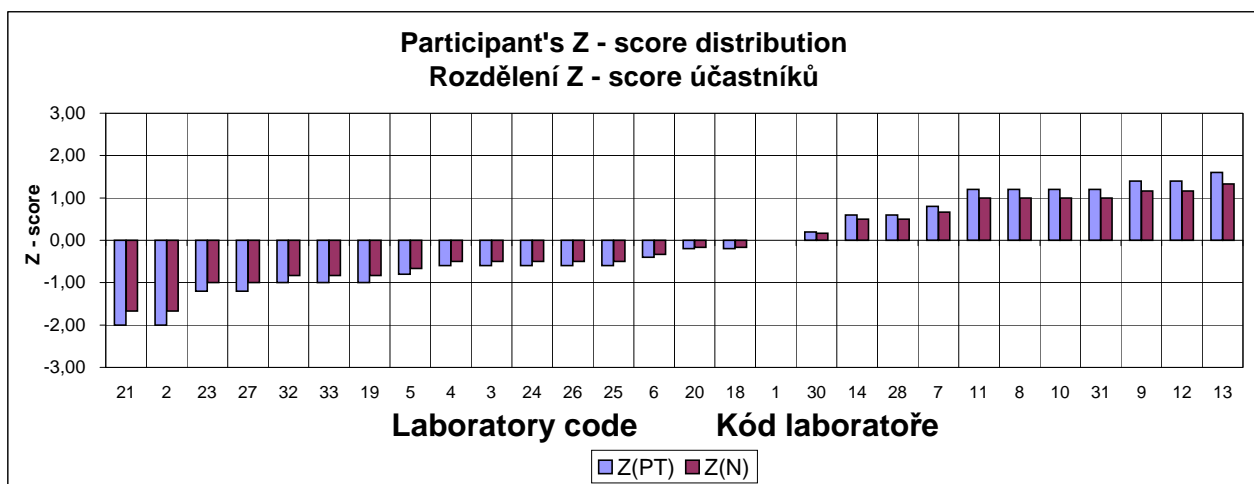

# PT 29/4A - S

## Results, statistical parameters and scoring


## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]         | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|--------|--------|--------|--------|---------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     | average       | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 16          |                  | -   |        |        |        |        |               |               |                       |                      |
| 18          |                  | -   |        |        |        |        |               |               |                       |                      |
| 21          |                  | -   |        |        |        |        |               |               |                       |                      |
| 23          |                  | -   |        |        |        |        |               |               |                       |                      |
| 29          |                  | -   |        |        |        |        |               |               |                       |                      |
| 4*          | IR               | 0,0044  | 0,0045 |        |        |        | <b>0,0044</b> |               | -4,77                 | -3,88                |
| 28          | IR               | 0,0078  | 0,0092 | 0,0086 | 0,0082 | 0,0079 | <b>0,0083</b> | 0,0007        | -1,77                 | -1,44                |
| 3           | AES              | 0,0082  | 0,0087 | 0,0087 | 0,0087 | 0,0083 | <b>0,0085</b> | 0,0003        | -1,62                 | -1,31                |
| 17          | IR               | 0,0090  | 0,0087 | 0,0083 | 0,0089 | 0,0094 | <b>0,0089</b> | 0,0005        | -1,31                 | -1,06                |
| 15          | IR               | 0,0094  | 0,0095 | 0,0091 | 0,0091 | 0,0092 | <b>0,0093</b> | 0,0002        | -1,00                 | -0,81                |
| 2           | XRF              | 0,0084  | 0,0096 | 0,0098 | 0,0090 | 0,0095 | <b>0,0093</b> | 0,0007        | -1,00                 | -0,81                |
| 34          | IR               | 0,0098  | 0,0094 | 0,0096 | 0,0091 | 0,0098 | <b>0,0095</b> | 0,0004        | -0,85                 | -0,69                |
| 7           | IR               | 0,0098  | 0,0098 | 0,0096 | 0,0097 | 0,0096 | <b>0,0097</b> | 0,0001        | -0,69                 | -0,56                |
| 33          | XRF              | 0,0101  | 0,0102 | 0,0098 | 0,0099 | 0,0101 | <b>0,0100</b> | 0,0002        | -0,46                 | -0,38                |
| 32          | AES              | 0,0098  | 0,0101 | 0,0104 | 0,0097 | 0,0100 | <b>0,0100</b> | 0,0003        | -0,46                 | -0,38                |
| 1           | AES              | 0,0095  | 0,0115 | 0,0082 | 0,0112 | 0,0100 | <b>0,0101</b> | 0,0017        | -0,38                 | -0,31                |
| 30          | IR               | 0,0100  | 0,0100 | 0,0100 | 0,0110 | 0,0100 | <b>0,0102</b> | 0,0006        | -0,31                 | -0,25                |
| 27          | XRF              | 0,0104  | 0,0101 | 0,0101 | 0,0103 | 0,0107 | <b>0,0103</b> | 0,0003        | -0,23                 | -0,19                |
| 9           | AES              | 0,0120  | 0,0100 | 0,0090 | 0,0090 | 0,0120 | <b>0,0104</b> | 0,0019        | -0,15                 | -0,13                |
| 22          | IR               | 0,0097  | 0,0104 | 0,0107 | 0,0107 | 0,0104 | <b>0,0104</b> | 0,0005        | -0,15                 | -0,13                |
| 19          | AES              | 0,0109  | 0,0110 | 0,0102 | 0,0099 | 0,0103 | <b>0,0105</b> | 0,0006        | -0,08                 | -0,06                |
| 8           | AES              | 0,0090  | 0,0130 | 0,0090 | 0,0090 | 0,0130 | <b>0,0106</b> | 0,0027        | 0,00                  | 0,00                 |
| 20          | AES              | 0,0105  | 0,0099 | 0,0117 | 0,0116 | 0,0101 | <b>0,0108</b> | 0,0010        | 0,15                  | 0,13                 |
| 10          | AES              | 0,0100  | 0,0090 | 0,0120 | 0,0110 | 0,0120 | <b>0,0108</b> | 0,0016        | 0,15                  | 0,13                 |
| 11          | AES              | 0,0100  | 0,0120 | 0,0110 | 0,0120 | 0,0100 | <b>0,0110</b> | 0,0012        | 0,31                  | 0,25                 |
| 13          | AES              | 0,0130  | 0,0090 | 0,0120 | 0,0100 | 0,0120 | <b>0,0112</b> | 0,0020        | 0,46                  | 0,38                 |
| 5           | AES              | 0,0102  | 0,0119 | 0,0120 | 0,0109 | 0,0118 | <b>0,0114</b> | 0,0010        | 0,62                  | 0,50                 |
| 12          | AES              | 0,0090  | 0,0130 | 0,0130 | 0,0090 | 0,0130 | <b>0,0114</b> | 0,0027        | 0,62                  | 0,50                 |
| 31          | AES              | 0,0110  | 0,0110 | 0,0131 | 0,0107 | 0,0135 | <b>0,0119</b> | 0,0016        | 1,00                  | 0,81                 |
| 24          | AES              | 0,0120  | 0,0121 | 0,0122 | 0,0120 | 0,0120 | <b>0,0121</b> | 0,0001        | 1,15                  | 0,94                 |
| 25          | AES              | 0,0130  | 0,0125 | 0,0122 | 0,0130 | 0,0125 | <b>0,0126</b> | 0,0004        | 1,54                  | 1,25                 |
| 6           | AES              | 0,0133  | 0,0146 | 0,0120 | 0,0117 | 0,0123 | <b>0,0128</b> | 0,0015        | 1,69                  | 1,38                 |
| 26          | AES              | 0,0130  | 0,0128 | 0,0125 | 0,0130 | 0,0128 | <b>0,0128</b> | 0,0003        | 1,69                  | 1,38                 |
| 14          | AES              | 0,0135  | 0,0153 | 0,0129 | 0,0100 | 0,0127 | <b>0,0129</b> | 0,0024        | 1,77                  | 1,44                 |

\* - result excluded as outlier

\* - výsledek vyloučen jako odlehlý

| n  | $\bar{X} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 28 | 0,0106                    | 0,0013                 | 0,0016                | 0,0005   |

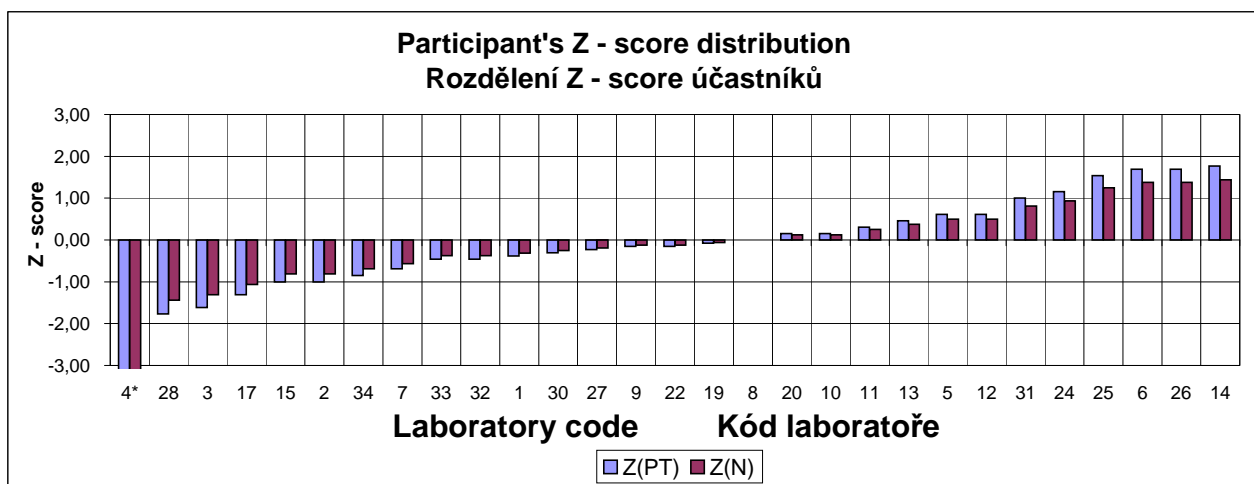




# PT 29/4A - Cu

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 15          |                  | -   |       |       |       |       |              |               |                       |                      |
| 16          |                  | -   |       |       |       |       |              |               |                       |                      |
| 21          |                  | -   |       |       |       |       |              |               |                       |                      |
| 22          |                  | -   |       |       |       |       |              |               |                       |                      |
| 34          |                  | -   |       |       |       |       |              |               |                       |                      |
| 17          | ICP              | 0,642   | 0,663 | 0,661 | 0,648 | 0,646 | <b>0,652</b> | 0,012         | -2,38                 | -2,38                |
| 29          | AES              | 0,668   | 0,669 | 0,665 | 0,667 | 0,669 | <b>0,668</b> | 0,002         | -1,37                 | -1,37                |
| 7           | AES              | 0,672   | 0,669 | 0,671 | 0,671 | 0,671 | <b>0,671</b> | 0,001         | -1,19                 | -1,19                |
| 13          | AES              | 0,672   | 0,675 | 0,674 | 0,678 | 0,673 | <b>0,674</b> | 0,003         | -1,00                 | -1,00                |
| 28          | ICP              | 0,694   | 0,671 | 0,651 | 0,684 | 0,677 | <b>0,675</b> | 0,020         | -0,94                 | -0,94                |
| 11          | AES              | 0,676   | 0,678 | 0,681 | 0,678 | 0,677 | <b>0,678</b> | 0,002         | -0,75                 | -0,75                |
| 8           | AES              | 0,683   | 0,678 | 0,677 | 0,680 | 0,678 | <b>0,679</b> | 0,003         | -0,69                 | -0,69                |
| 30          | AES              | 0,680   | 0,680 | 0,680 | 0,680 | 0,680 | <b>0,680</b> | 0,000         | -0,62                 | -0,62                |
| 23          | ICP              | 0,679   | 0,680 | 0,681 | 0,680 | 0,681 | <b>0,680</b> | 0,001         | -0,62                 | -0,62                |
| 10          | AES              | 0,683   | 0,679 | 0,680 | 0,684 | 0,677 | <b>0,681</b> | 0,004         | -0,56                 | -0,56                |
| 12          | AES              | 0,682   | 0,683 | 0,682 | 0,677 | 0,681 | <b>0,681</b> | 0,003         | -0,56                 | -0,56                |
| 9           | AES              | 0,682   | 0,682 | 0,680 | 0,679 | 0,685 | <b>0,682</b> | 0,003         | -0,50                 | -0,50                |
| 1           | AES              | 0,683   | 0,686 | 0,687 | 0,696 | 0,694 | <b>0,689</b> | 0,007         | -0,06                 | -0,06                |
| 20          | AES              | 0,692   | 0,691 | 0,692 | 0,689 | 0,688 | <b>0,690</b> | 0,003         | 0,00                  | 0,00                 |
| 19          | AES              | 0,688   | 0,706 | 0,695 | 0,688 | 0,678 | <b>0,691</b> | 0,013         | 0,06                  | 0,06                 |
| 2           | XRF              | 0,686   | 0,696 | 0,688 | 0,694 | 0,693 | <b>0,691</b> | 0,005         | 0,06                  | 0,06                 |
| 5           | AES              | 0,697   | 0,685 | 0,691 | 0,693 | 0,694 | <b>0,692</b> | 0,006         | 0,13                  | 0,13                 |
| 27          | XRF              | 0,692   | 0,689 | 0,692 | 0,701 | 0,690 | <b>0,693</b> | 0,006         | 0,19                  | 0,19                 |
| 32          | AES              | 0,699   | 0,692 | 0,694 | 0,696 | 0,694 | <b>0,695</b> | 0,003         | 0,31                  | 0,31                 |
| 3           | AES              | 0,700   | 0,700 | 0,700 | 0,700 | 0,699 | <b>0,700</b> | 0,001         | 0,63                  | 0,63                 |
| 4           | AES              | 0,700   | 0,700 | 0,700 |       |       | <b>0,700</b> | 0,000         | 0,63                  | 0,63                 |
| 26          | AES              | 0,701   | 0,702 | 0,703 | 0,701 | 0,702 | <b>0,702</b> | 0,001         | 0,75                  | 0,75                 |
| 25          | AES              | 0,704   | 0,703 | 0,704 | 0,701 | 0,704 | <b>0,703</b> | 0,002         | 0,81                  | 0,81                 |
| 24          | AES              | 0,705   | 0,702 | 0,705 | 0,702 | 0,704 | <b>0,704</b> | 0,002         | 0,88                  | 0,88                 |
| 33          | XRF              | 0,703   | 0,706 | 0,705 | 0,703 | 0,703 | <b>0,704</b> | 0,002         | 0,88                  | 0,88                 |
| 6           | AES              | 0,708   | 0,704 | 0,705 | 0,705 | 0,702 | <b>0,705</b> | 0,003         | 0,94                  | 0,94                 |
| 14          | AES              | 0,690   | 0,724 | 0,735 | 0,695 | 0,707 | <b>0,710</b> | 0,024         | 1,25                  | 1,25                 |
| 31          | AES              | 0,768   | 0,736 | 0,666 | 0,703 | 0,696 | <b>0,714</b> | 0,049         | 1,50                  | 1,50                 |
| 18          | AES              | 0,719   | 0,730 | 0,728 | 0,722 | 0,723 | <b>0,724</b> | 0,006         | 2,13                  | 2,13                 |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 29 | 0,690                     | 0,016                  | 0,016                 | 0,006    |

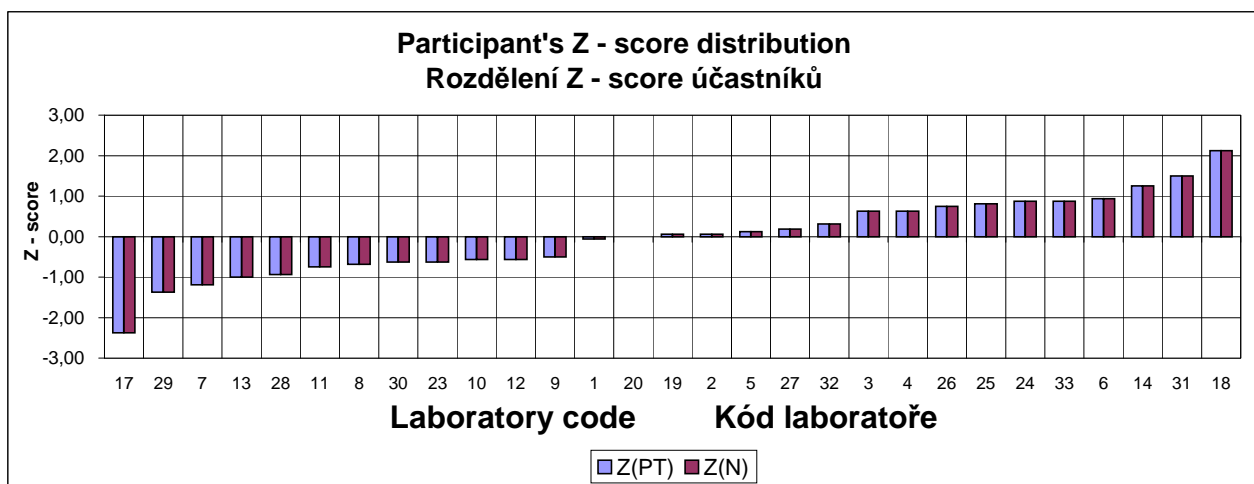


PT 29/4A - Cr

Results, statistical parameters and scoring

Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 4           | AES              | 0,650   | 0,630 | 0,640 |       |       | <b>0,640</b>     | 0,025                  | -1,61                                    | -1,71                                  |
| 17          | ICP              | 0,622   | 0,650 | 0,648 | 0,637 | 0,648 | <b>0,641</b>     | 0,015                  | -1,56                                    | -1,65                                  |
| 6           | AES              | 0,650   | 0,639 | 0,648 | 0,654 | 0,636 | <b>0,645</b>     | 0,009                  | -1,33                                    | -1,41                                  |
| 32          | AES              | 0,648   | 0,653 | 0,654 | 0,651 | 0,647 | <b>0,651</b>     | 0,004                  | -1,00                                    | -1,06                                  |
| 1           | AES              | 0,652   | 0,655 | 0,657 | 0,653 | 0,650 | <b>0,653</b>     | 0,003                  | -0,89                                    | -0,94                                  |
| 31          | AES              | 0,657   | 0,657 | 0,654 | 0,654 | 0,655 | <b>0,655</b>     | 0,002                  | -0,78                                    | -0,82                                  |
| 14          | AES              | 0,657   | 0,657 | 0,654 | 0,654 | 0,655 | <b>0,655</b>     | 0,002                  | -0,78                                    | -0,82                                  |
| 5           | AES              | 0,652   | 0,652 | 0,658 | 0,656 | 0,656 | <b>0,655</b>     | 0,003                  | -0,78                                    | -0,82                                  |
| 7           | AES              | 0,658   | 0,659 | 0,658 | 0,658 | 0,658 | <b>0,658</b>     | 0,001                  | -0,61                                    | -0,65                                  |
| 18          | AES              | 0,665   | 0,656 | 0,659 | 0,673 | 0,652 | <b>0,661</b>     | 0,010                  | -0,44                                    | -0,47                                  |
| 20          | AES              | 0,662   | 0,663 | 0,660 | 0,661 | 0,663 | <b>0,662</b>     | 0,002                  | -0,39                                    | -0,41                                  |
| 21          | Titrimetric      | 0,651   | 0,665 | 0,658 | 0,667 | 0,669 | <b>0,662</b>     | 0,009                  | -0,39                                    | -0,41                                  |
| 2           | XRF              | 0,660   | 0,667 | 0,664 | 0,665 | 0,661 | <b>0,663</b>     | 0,004                  | -0,33                                    | -0,35                                  |
| 29          | AES              | 0,666   | 0,662 | 0,660 | 0,670 | 0,665 | <b>0,665</b>     | 0,005                  | -0,22                                    | -0,24                                  |
| 23          | ICP              | 0,668   | 0,670 | 0,660 | 0,665 | 0,668 | <b>0,666</b>     | 0,005                  | -0,17                                    | -0,18                                  |
| 33          | XRF              | 0,667   | 0,668 | 0,671 | 0,670 | 0,669 | <b>0,669</b>     | 0,002                  | 0,00                                     | 0,00                                   |
| 3           | AES              | 0,675   | 0,657 | 0,676 | 0,671 | 0,673 | <b>0,670</b>     | 0,010                  | 0,06                                     | 0,06                                   |
| 10          | AES              | 0,668   | 0,676 | 0,672 | 0,670 | 0,663 | <b>0,670</b>     | 0,006                  | 0,06                                     | 0,06                                   |
| 11          | AES              | 0,672   | 0,671 | 0,670 | 0,673 | 0,670 | <b>0,671</b>     | 0,002                  | 0,11                                     | 0,12                                   |
| 13          | AES              | 0,671   | 0,673 | 0,672 | 0,672 | 0,674 | <b>0,672</b>     | 0,001                  | 0,17                                     | 0,18                                   |
| 9           | AES              | 0,670   | 0,674 | 0,672 | 0,674 | 0,672 | <b>0,672</b>     | 0,002                  | 0,17                                     | 0,18                                   |
| 12          | AES              | 0,668   | 0,673 | 0,674 | 0,675 | 0,672 | <b>0,672</b>     | 0,003                  | 0,17                                     | 0,18                                   |
| 8           | AES              | 0,671   | 0,671 | 0,672 | 0,671 | 0,678 | <b>0,673</b>     | 0,004                  | 0,22                                     | 0,24                                   |
| 19          | AES              | 0,683   | 0,684 | 0,682 | 0,682 | 0,679 | <b>0,682</b>     | 0,002                  | 0,72                                     | 0,76                                   |
| 30          | AES              | 0,680   | 0,680 | 0,680 | 0,680 | 0,690 | <b>0,682</b>     | 0,006                  | 0,72                                     | 0,76                                   |
| 28          | ICP              | 0,681   | 0,690 | 0,692 | 0,691 | 0,679 | <b>0,687</b>     | 0,008                  | 1,00                                     | 1,06                                   |
| 27          | XRF              | 0,700   | 0,696 | 0,696 | 0,699 | 0,697 | <b>0,698</b>     | 0,002                  | 1,61                                     | 1,71                                   |
| 24          | AES              | 0,703   | 0,699 | 0,698 | 0,699 | 0,699 | <b>0,700</b>     | 0,002                  | 1,72                                     | 1,82                                   |
| 26          | AES              | 0,701   | 0,700 | 0,702 | 0,701 | 0,702 | <b>0,701</b>     | 0,001                  | 1,78                                     | 1,88                                   |
| 25          | AES              | 0,713   | 0,711 | 0,710 | 0,711 | 0,713 | <b>0,712</b>     | 0,002                  | 2,39                                     | 2,53                                   |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 30 | 0,669                     | 0,018                  | 0,017                 | 0,007    |

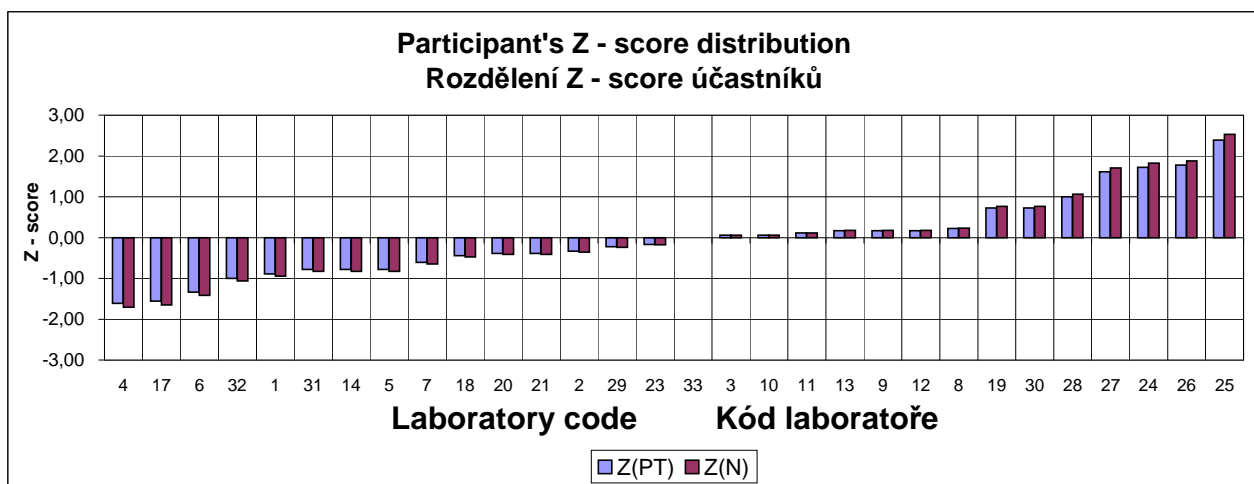


# PT 29/4A - Ni

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 23          | ICP              | 0,989   | 0,990 | 0,995 | 0,987 | 0,998 | <b>0,992</b>     | 0,006                  | -1,84                                    | -1,59                                  |
| 1           | AES              | 0,998   | 0,995 | 0,999 | 0,992 | 0,997 | <b>0,996</b>     | 0,003                  | -1,63                                    | -1,41                                  |
| 21          | Gravimetric      | 1,002   | 0,999 | 0,990 | 0,997 | 1,000 | <b>0,998</b>     | 0,006                  | -1,53                                    | -1,32                                  |
| 5           | AES              | 1,002   | 0,992 | 1,008 | 1,004 | 1,009 | <b>1,003</b>     | 0,008                  | -1,26                                    | -1,09                                  |
| 20          | AES              | 1,010   | 1,012 | 1,016 | 1,008 | 1,007 | <b>1,011</b>     | 0,004                  | -0,84                                    | -0,73                                  |
| 28          | ICP              | 1,006   | 0,999 | 1,031 | 1,012 | 1,010 | <b>1,012</b>     | 0,015                  | -0,79                                    | -0,68                                  |
| 8           | AES              | 1,016   | 1,015 | 1,013 | 1,015 | 1,013 | <b>1,014</b>     | 0,002                  | -0,68                                    | -0,59                                  |
| 12          | AES              | 1,016   | 1,018 | 1,015 | 1,011 | 1,011 | <b>1,014</b>     | 0,004                  | -0,68                                    | -0,59                                  |
| 13          | AES              | 1,014   | 1,014 | 1,013 | 1,016 | 1,011 | <b>1,014</b>     | 0,002                  | -0,68                                    | -0,59                                  |
| 10          | AES              | 1,018   | 1,017 | 1,014 | 1,020 | 1,013 | <b>1,016</b>     | 0,004                  | -0,58                                    | -0,50                                  |
| 11          | AES              | 1,016   | 1,018 | 1,019 | 1,017 | 1,017 | <b>1,017</b>     | 0,001                  | -0,53                                    | -0,45                                  |
| 9           | AES              | 1,020   | 1,018 | 1,018 | 1,017 | 1,025 | <b>1,020</b>     | 0,004                  | -0,37                                    | -0,32                                  |
| 19          | AES              | 1,020   | 1,020 | 1,020 | 1,020 | 1,020 | <b>1,020</b>     | 0,000                  | -0,37                                    | -0,32                                  |
| 32          | AES              | 1,018   | 1,026 | 1,023 | 1,027 | 1,011 | <b>1,021</b>     | 0,008                  | -0,32                                    | -0,27                                  |
| 2           | XRF              | 1,021   | 1,026 | 1,025 | 1,024 | 1,021 | <b>1,023</b>     | 0,003                  | -0,21                                    | -0,18                                  |
| 4           | AES              | 1,010   | 1,040 | 1,020 |       |       | <b>1,023</b>     | 0,038                  | -0,21                                    | -0,18                                  |
| 29          | AES              | 1,032   | 1,026 | 1,028 | 1,034 | 1,027 | <b>1,029</b>     | 0,004                  | 0,11                                     | 0,09                                   |
| 14          | AES              | 1,026   | 1,030 | 1,037 | 1,034 | 1,036 | <b>1,033</b>     | 0,006                  | 0,32                                     | 0,27                                   |
| 30          | AES              | 1,030   | 1,030 | 1,030 | 1,040 | 1,040 | <b>1,034</b>     | 0,007                  | 0,37                                     | 0,32                                   |
| 31          | AES              | 1,023   | 1,015 | 1,052 | 1,030 | 1,049 | <b>1,034</b>     | 0,020                  | 0,37                                     | 0,32                                   |
| 7           | AES              | 1,037   | 1,034 | 1,034 | 1,036 | 1,034 | <b>1,035</b>     | 0,002                  | 0,42                                     | 0,36                                   |
| 6           | AES              | 1,018   | 1,047 | 1,030 | 1,034 | 1,051 | <b>1,036</b>     | 0,017                  | 0,47                                     | 0,41                                   |
| 17          | ICP              | 1,054   | 1,034 | 1,045 | 1,067 | 1,033 | <b>1,047</b>     | 0,018                  | 1,05                                     | 0,91                                   |
| 24          | AES              | 1,046   | 1,048 | 1,042 | 1,050 | 1,050 | <b>1,047</b>     | 0,004                  | 1,05                                     | 0,91                                   |
| 33          | XRF              | 1,049   | 1,047 | 1,045 | 1,051 | 1,050 | <b>1,048</b>     | 0,003                  | 1,11                                     | 0,95                                   |
| 26          | AES              | 1,052   | 1,054 | 1,052 | 1,054 | 1,050 | <b>1,052</b>     | 0,002                  | 1,32                                     | 1,14                                   |
| 27          | XRF              | 1,057   | 1,050 | 1,058 | 1,058 | 1,045 | <b>1,054</b>     | 0,007                  | 1,42                                     | 1,23                                   |
| 25          | AES              | 1,057   | 1,056 | 1,054 | 1,056 | 1,054 | <b>1,055</b>     | 0,002                  | 1,47                                     | 1,27                                   |
| 3           | AES              | 1,051   | 1,056 | 1,060 | 1,062 | 1,054 | <b>1,057</b>     | 0,006                  | 1,58                                     | 1,36                                   |
| 18          | AES              | 1,070   | 1,045 | 1,077 | 1,075 | 1,050 | <b>1,063</b>     | 0,018                  | 1,89                                     | 1,64                                   |

| n  | $\bar{X} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 30 | 1,027                     | 0,019                  | 0,022                 | 0,007    |

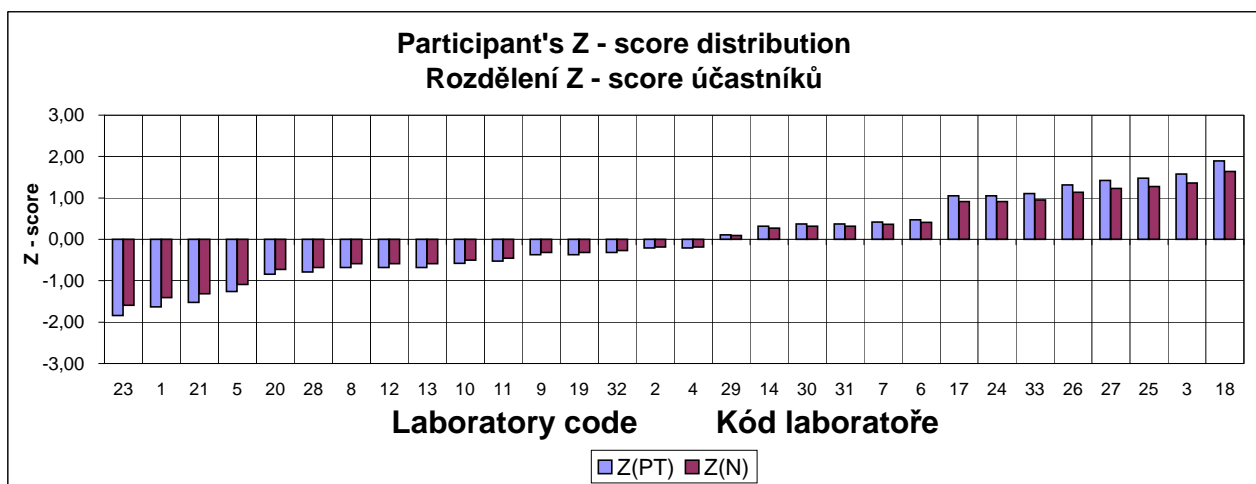

# PT 29/4A - AI

## Results, statistical parameters and scoring


## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|--------|--------|--------|--------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     |                  |                        |  |  |
| 1           |                  | -   |        |        |        |        |                  |                        |  |  |
| 2           |                  | -   |        |        |        |        |                  |                        |  |  |
| 3           |                  | -   |        |        |        |        |                  |                        |  |  |
| 15          |                  | -   |        |        |        |        |                  |                        |  |  |
| 16          |                  | -   |        |        |        |        |                  |                        |  |  |
| 21          |                  | -   |        |        |        |        |                  |                        |  |  |
| 22          |                  | -   |        |        |        |        |                  |                        |  |  |
| 24          |                  | -   |        |        |        |        |                  |                        |  |  |
| 25          |                  | -   |        |        |        |        |                  |                        |  |  |
| 26          |                  | -   |        |        |        |        |                  |                        |  |  |
| 27          |                  | -   |        |        |        |        |                  |                        |  |  |
| 33          |                  | -   |        |        |        |        |                  |                        |  |  |
| 34          |                  | -   |        |        |        |        |                  |                        |  |  |
| 28          | ICP              | 0,0209  | 0,0213 | 0,0212 | 0,0202 | 0,0215 | <b>0,0210</b>    | 0,0006                 | -1,43                                    | -1,15                                  |
| 31          | AES              | 0,0223  | 0,0220 | 0,0215 | 0,0212 | 0,0211 | <b>0,0216</b>    | 0,0006                 | -1,14                                    | -0,92                                  |
| 19          | AES              | 0,0216  | 0,0220 | 0,0215 | 0,0217 | 0,0210 | <b>0,0216</b>    | 0,0005                 | -1,14                                    | -0,92                                  |
| 5           | AES              | 0,0220  | 0,0210 | 0,0220 | 0,0220 | 0,0220 | <b>0,0218</b>    | 0,0006                 | -1,05                                    | -0,85                                  |
| 20          | AES              | 0,0220  | 0,0219 | 0,0221 | 0,0220 | 0,0221 | <b>0,0220</b>    | 0,0001                 | -0,95                                    | -0,77                                  |
| 18          | AES              | 0,0215  | 0,0225 | 0,0228 | 0,0229 | 0,0223 | <b>0,0224</b>    | 0,0007                 | -0,76                                    | -0,62                                  |
| 6           | AES              | 0,0223  | 0,0228 | 0,0231 | 0,0235 | 0,0231 | <b>0,0230</b>    | 0,0006                 | -0,48                                    | -0,38                                  |
| 11          | AES              | 0,0240  | 0,0240 | 0,0240 | 0,0240 | 0,0230 | <b>0,0238</b>    | 0,0006                 | -0,10                                    | -0,08                                  |
| 17          | ICP              | 0,0229  | 0,0243 | 0,0233 | 0,0245 | 0,0238 | <b>0,0238</b>    | 0,0008                 | -0,10                                    | -0,08                                  |
| 32          | AES              | 0,0241  | 0,0238 | 0,0229 | 0,0242 | 0,0247 | <b>0,0239</b>    | 0,0008                 | -0,05                                    | -0,04                                  |
| 9           | AES              | 0,0240  | 0,0240 | 0,0240 | 0,0240 | 0,0240 | <b>0,0240</b>    | 0,0000                 | 0,00                                     | 0,00                                   |
| 13          | AES              | 0,0240  | 0,0240 | 0,0240 | 0,0240 | 0,0240 | <b>0,0240</b>    | 0,0000                 | 0,00                                     | 0,00                                   |
| 14          | AES              | 0,0237  | 0,0239 | 0,0243 | 0,0243 | 0,0241 | <b>0,0241</b>    | 0,0003                 | 0,05                                     | 0,04                                   |
| 8           | AES              | 0,0240  | 0,0250 | 0,0240 | 0,0240 | 0,0240 | <b>0,0242</b>    | 0,0006                 | 0,10                                     | 0,08                                   |
| 12          | AES              | 0,0250  | 0,0240 | 0,0240 | 0,0250 | 0,0250 | <b>0,0246</b>    | 0,0007                 | 0,29                                     | 0,23                                   |
| 4           | AES              | 0,0250  | 0,0250 | 0,0250 |        |        | <b>0,0250</b>    | 0,0000                 | 0,48                                     | 0,38                                   |
| 10          | AES              | 0,0260  | 0,0260 | 0,0280 | 0,0270 | 0,0260 | <b>0,0266</b>    | 0,0011                 | 1,24                                     | 1,00                                   |
| 29          | AES              | 0,0270  | 0,0270 | 0,0270 | 0,0270 | 0,0270 | <b>0,0270</b>    | 0,0000                 | 1,43                                     | 1,15                                   |
| 7           | AES              | 0,0277  | 0,0279 | 0,0279 | 0,0278 | 0,0273 | <b>0,0277</b>    | 0,0003                 | 1,76                                     | 1,42                                   |
| 23          | ICP              | 0,0300  | 0,0280 | 0,0280 | 0,0270 | 0,0300 | <b>0,0286</b>    | 0,0017                 | 2,19                                     | 1,77                                   |
| 30*         | AES              | 0,0320  | 0,0320 | 0,0320 | 0,0320 | 0,0320 | <b>0,0320</b>    | 0,0000                 | 3,81                                     | 3,08                                   |

\* - result excluded as outlier

\* - výsledek vyloučen jako odlehlý

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 20 | 0,0240                    | 0,0021                 | 0,0026                | 0,0010   |

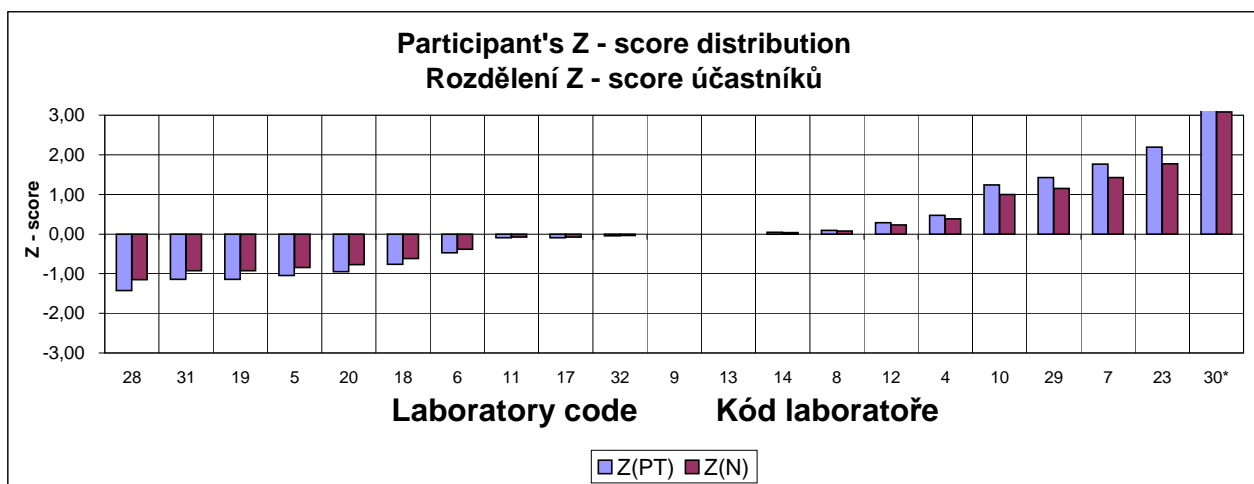


# PT 29/4A - Mo

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 3           |                  | -   |       |       |       |       |              |               |                       |                      |
| 15          |                  | -   |       |       |       |       |              |               |                       |                      |
| 16          |                  | -   |       |       |       |       |              |               |                       |                      |
| 22          |                  | -   |       |       |       |       |              |               |                       |                      |
| 34          |                  | -   |       |       |       |       |              |               |                       |                      |
| 19          | AES              | 0,051   | 0,050 | 0,050 | 0,046 | 0,044 | <b>0,048</b> | 0,004         | -1,75                 | -1,71                |
| 23          | ICP              | 0,047   | 0,050 | 0,051 | 0,048 | 0,048 | <b>0,049</b> | 0,002         | -1,50                 | -1,46                |
| 30          | AES              | 0,050   | 0,050 | 0,050 | 0,050 | 0,050 | <b>0,050</b> | 0,000         | -1,25                 | -1,22                |
| 31          | AES              | 0,053   | 0,051 | 0,051 | 0,049 | 0,051 | <b>0,051</b> | 0,002         | -1,00                 | -0,98                |
| 4           | AES              | 0,054   | 0,051 | 0,052 |       |       | <b>0,052</b> | 0,004         | -0,75                 | -0,73                |
| 5           | AES              | 0,054   | 0,051 | 0,054 | 0,053 | 0,050 | <b>0,052</b> | 0,002         | -0,75                 | -0,73                |
| 7           | AES              | 0,051   | 0,051 | 0,052 | 0,052 | 0,052 | <b>0,052</b> | 0,001         | -0,75                 | -0,73                |
| 14          | AES              | 0,051   | 0,052 | 0,051 | 0,051 | 0,053 | <b>0,052</b> | 0,001         | -0,75                 | -0,73                |
| 25          | AES              | 0,052   | 0,054 | 0,052 | 0,053 | 0,054 | <b>0,053</b> | 0,001         | -0,50                 | -0,49                |
| 1           | AES              | 0,054   | 0,054 | 0,054 | 0,054 | 0,055 | <b>0,054</b> | 0,001         | -0,25                 | -0,24                |
| 29          | AES              | 0,054   | 0,054 | 0,054 | 0,054 | 0,054 | <b>0,054</b> | 0,000         | -0,25                 | -0,24                |
| 26          | AES              | 0,056   | 0,054 | 0,056 | 0,055 | 0,056 | <b>0,055</b> | 0,001         | 0,00                  | 0,00                 |
| 28          | ICP              | 0,055   | 0,053 | 0,058 | 0,054 | 0,053 | <b>0,055</b> | 0,003         | 0,00                  | 0,00                 |
| 32          | AES              | 0,054   | 0,055 | 0,055 | 0,056 | 0,056 | <b>0,055</b> | 0,001         | 0,00                  | 0,00                 |
| 6           | AES              | 0,057   | 0,056 | 0,056 | 0,055 | 0,054 | <b>0,056</b> | 0,001         | 0,25                  | 0,24                 |
| 17          | ICP              | 0,056   | 0,056 | 0,056 | 0,056 | 0,055 | <b>0,056</b> | 0,001         | 0,25                  | 0,24                 |
| 27          | XRF              | 0,056   | 0,057 | 0,057 | 0,057 | 0,055 | <b>0,056</b> | 0,001         | 0,25                  | 0,24                 |
| 2           | XRF              | 0,055   | 0,057 | 0,057 | 0,057 | 0,055 | <b>0,056</b> | 0,001         | 0,25                  | 0,24                 |
| 11          | AES              | 0,058   | 0,057 | 0,057 | 0,057 | 0,057 | <b>0,057</b> | 0,001         | 0,50                  | 0,49                 |
| 24          | AES              | 0,057   | 0,056 | 0,057 | 0,056 | 0,057 | <b>0,057</b> | 0,001         | 0,50                  | 0,49                 |
| 13          | AES              | 0,057   | 0,057 | 0,057 | 0,058 | 0,058 | <b>0,057</b> | 0,001         | 0,50                  | 0,49                 |
| 18          | AES              | 0,059   | 0,057 | 0,059 | 0,057 | 0,058 | <b>0,058</b> | 0,001         | 0,75                  | 0,73                 |
| 9           | AES              | 0,057   | 0,058 | 0,058 | 0,057 | 0,058 | <b>0,058</b> | 0,001         | 0,75                  | 0,73                 |
| 33          | XRF              | 0,059   | 0,058 | 0,060 | 0,060 | 0,060 | <b>0,059</b> | 0,001         | 1,00                  | 0,98                 |
| 12          | AES              | 0,061   | 0,060 | 0,060 | 0,061 | 0,060 | <b>0,060</b> | 0,001         | 1,25                  | 1,22                 |
| 8           | AES              | 0,060   | 0,060 | 0,060 | 0,060 | 0,060 | <b>0,060</b> | 0,000         | 1,25                  | 1,22                 |
| 10          | AES              | 0,060   | 0,060 | 0,060 | 0,060 | 0,061 | <b>0,060</b> | 0,001         | 1,25                  | 1,22                 |
| 20          | AES              | 0,060   | 0,060 | 0,060 | 0,060 | 0,060 | <b>0,060</b> | 0,000         | 1,25                  | 1,22                 |
| 21          | Photometric      | 0,061   | 0,061 | 0,061 | 0,061 | 0,061 | <b>0,061</b> | 0,000         | 1,50                  | 1,46                 |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 29 | 0,055                     | 0,004                  | 0,004                 | 0,002    |

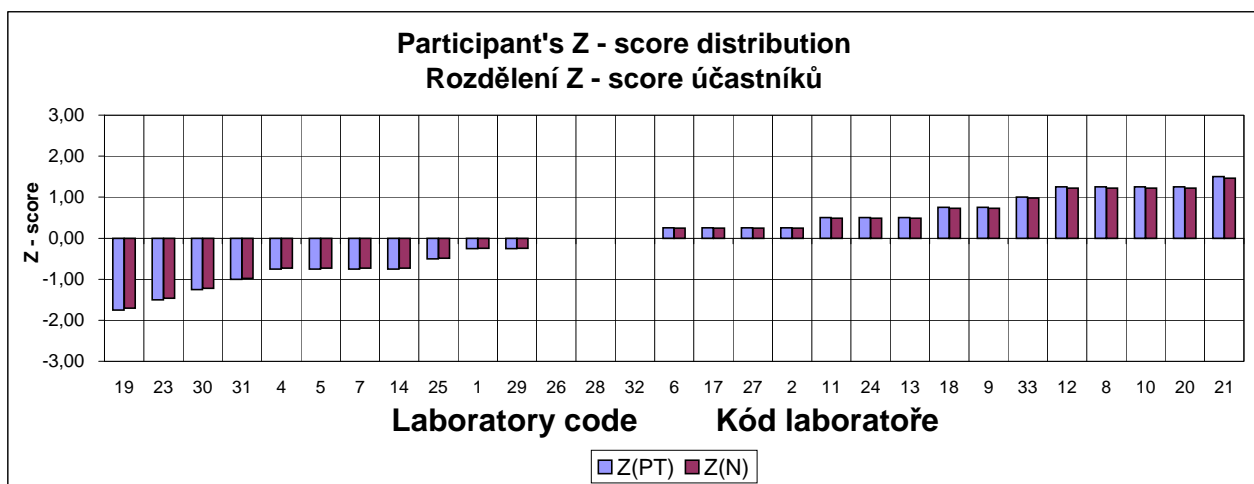


# PT 29/4A - Mg

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 1           |                  | -   |       |       |       |       |              |               |                       |                      |
| 2           |                  | -   |       |       |       |       |              |               |                       |                      |
| 15          |                  | -   |       |       |       |       |              |               |                       |                      |
| 16          |                  | -   |       |       |       |       |              |               |                       |                      |
| 21          |                  | -   |       |       |       |       |              |               |                       |                      |
| 22          |                  | -   |       |       |       |       |              |               |                       |                      |
| 27          |                  | -   |       |       |       |       |              |               |                       |                      |
| 28          |                  | -   |       |       |       |       |              |               |                       |                      |
| 29          |                  | -   |       |       |       |       |              |               |                       |                      |
| 33          |                  | -   |       |       |       |       |              |               |                       |                      |
| 34          |                  | -   |       |       |       |       |              |               |                       |                      |
| 18          | AES              | 0,040   | 0,040 | 0,043 | 0,040 | 0,043 | <b>0,041</b> | 0,002         | -1,75                 | -1,40                |
| 31          | AES              | 0,041   | 0,042 | 0,044 | 0,041 | 0,045 | <b>0,043</b> | 0,002         | -1,25                 | -1,00                |
| 14          | AES              | 0,044   | 0,037 | 0,050 | 0,048 | 0,042 | <b>0,044</b> | 0,006         | -1,00                 | -0,80                |
| 17          | ICP              | 0,043   | 0,043 | 0,043 | 0,045 | 0,045 | <b>0,044</b> | 0,001         | -1,00                 | -0,80                |
| 23          | ICP              | 0,042   | 0,046 | 0,046 | 0,045 | 0,043 | <b>0,044</b> | 0,002         | -1,00                 | -0,80                |
| 19          | AES              | 0,043   | 0,048 | 0,043 | 0,048 | 0,044 | <b>0,045</b> | 0,003         | -0,75                 | -0,60                |
| 7           | AES              | 0,044   | 0,047 | 0,046 | 0,047 | 0,046 | <b>0,046</b> | 0,001         | -0,50                 | -0,40                |
| 8           | AES              | 0,044   | 0,045 | 0,045 | 0,049 | 0,045 | <b>0,046</b> | 0,002         | -0,50                 | -0,40                |
| 4           | AES              | 0,043   | 0,050 | 0,045 |       |       | <b>0,046</b> | 0,009         | -0,50                 | -0,40                |
| 20          | AES              | 0,047   | 0,047 | 0,048 | 0,047 | 0,047 | <b>0,047</b> | 0,001         | -0,25                 | -0,20                |
| 24          | AES              | 0,046   | 0,047 | 0,046 | 0,047 | 0,047 | <b>0,047</b> | 0,001         | -0,25                 | -0,20                |
| 13          | AES              | 0,050   | 0,047 | 0,049 | 0,046 | 0,049 | <b>0,048</b> | 0,002         | 0,00                  | 0,00                 |
| 3           | AES              | 0,047   | 0,047 | 0,047 | 0,046 | 0,051 | <b>0,048</b> | 0,002         | 0,00                  | 0,00                 |
| 11          | AES              | 0,051   | 0,049 | 0,048 | 0,050 | 0,048 | <b>0,049</b> | 0,002         | 0,25                  | 0,20                 |
| 10          | AES              | 0,050   | 0,045 | 0,052 | 0,046 | 0,054 | <b>0,049</b> | 0,005         | 0,25                  | 0,20                 |
| 9           | AES              | 0,049   | 0,048 | 0,046 | 0,052 | 0,048 | <b>0,049</b> | 0,003         | 0,25                  | 0,20                 |
| 12          | AES              | 0,047   | 0,049 | 0,048 | 0,053 | 0,050 | <b>0,049</b> | 0,003         | 0,25                  | 0,20                 |
| 6           | AES              | 0,056   | 0,051 | 0,051 | 0,044 | 0,047 | <b>0,050</b> | 0,006         | 0,50                  | 0,40                 |
| 26          | AES              | 0,050   | 0,049 | 0,050 | 0,051 | 0,050 | <b>0,050</b> | 0,001         | 0,50                  | 0,40                 |
| 30          | AES              | 0,050   | 0,052 | 0,054 | 0,055 | 0,047 | <b>0,052</b> | 0,004         | 1,00                  | 0,80                 |
| 25          | AES              | 0,053   | 0,053 | 0,054 | 0,052 | 0,052 | <b>0,053</b> | 0,001         | 1,25                  | 1,00                 |
| 32          | AES              | 0,056   | 0,053 | 0,055 | 0,057 | 0,058 | <b>0,056</b> | 0,002         | 2,00                  | 1,60                 |
| 5           | AES              | 0,059   | 0,061 | 0,060 | 0,053 | 0,051 | <b>0,057</b> | 0,006         | 2,25                  | 1,80                 |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 23 | 0,048                     | 0,004                  | 0,005                 | 0,002    |

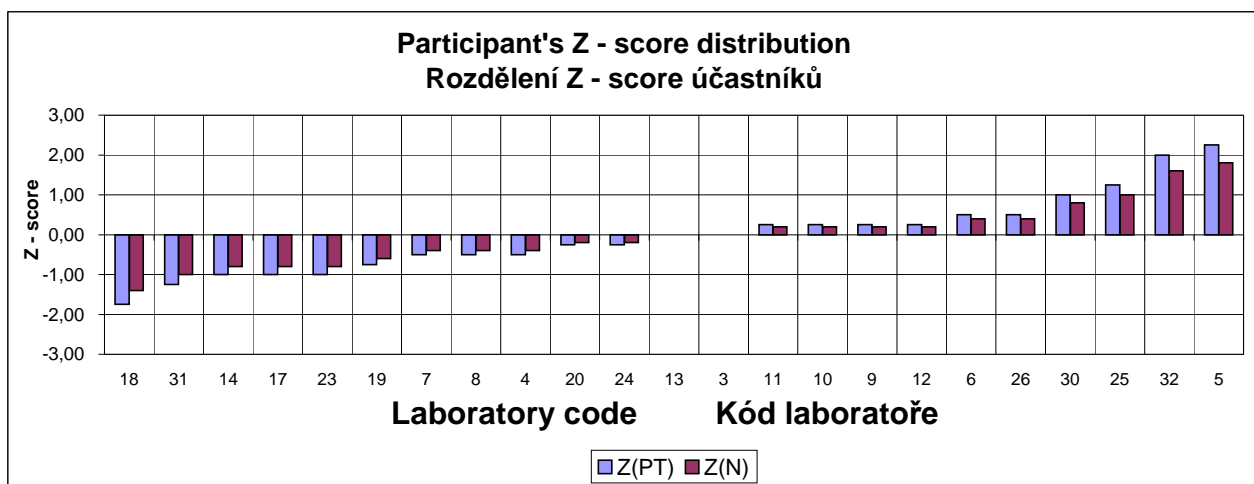


# PT 29/4A - Ce

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 1           |                  | -   |       |       |       |       |                  |                        |  |  |
| 2           |                  | -   |       |       |       |       |                  |                        |  |  |
| 3           |                  | -   |       |       |       |       |                  |                        |  |  |
| 5           |                  | -   |       |       |       |       |                  |                        |  |  |
| 9           |                  | -   |       |       |       |       |                  |                        |  |  |
| 11          |                  | -   |       |       |       |       |                  |                        |  |  |
| 13          |                  | -   |       |       |       |       |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 18          |                  | -   |       |       |       |       |                  |                        |  |  |
| 21          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 23          |                  | -   |       |       |       |       |                  |                        |  |  |
| 24          |                  | -   |       |       |       |       |                  |                        |  |  |
| 25          |                  | -   |       |       |       |       |                  |                        |  |  |
| 26          |                  | -   |       |       |       |       |                  |                        |  |  |
| 27          |                  | -   |       |       |       |       |                  |                        |  |  |
| 28          |                  | -   |       |       |       |       |                  |                        |  |  |
| 29          |                  | -   |       |       |       |       |                  |                        |  |  |
| 33          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 17          | ICP              | 0,030   | 0,031 | 0,031 | 0,030 | 0,030 | <b>0,030</b>     | 0,000                  | -1,33                                    | -0,67                                  |
| 31          | AES              | 0,026   | 0,031 | 0,029 | 0,030 | 0,033 | <b>0,030</b>     | 0,003                  | -1,33                                    | -0,67                                  |
| 19          | AES              | 0,031   | 0,031 | 0,036 | 0,032 | 0,026 | <b>0,031</b>     | 0,004                  | -1,00                                    | -0,50                                  |
| 14          | AES              | 0,028   | 0,032 | 0,032 | 0,026 | 0,036 | <b>0,031</b>     | 0,005                  | -1,00                                    | -0,50                                  |
| 8           | AES              | 0,027   | 0,035 | 0,031 | 0,032 | 0,033 | <b>0,032</b>     | 0,004                  | -0,67                                    | -0,33                                  |
| 4           | AES              | 0,033   | 0,030 | 0,035 |       |       | <b>0,033</b>     | 0,006                  | -0,33                                    | -0,17                                  |
| 20          | AES              | 0,034   | 0,033 | 0,034 | 0,035 | 0,036 | <b>0,034</b>     | 0,001                  | 0,00                                     | 0,00                                   |
| 7           | AES              | 0,032   | 0,035 | 0,034 | 0,034 | 0,033 | <b>0,034</b>     | 0,001                  | 0,00                                     | 0,00                                   |
| 32          | AES              | 0,036   | 0,038 | 0,036 | 0,035 | 0,034 | <b>0,036</b>     | 0,002                  | 0,67                                     | 0,33                                   |
| 30          | AES              | 0,036   | 0,035 | 0,041 | 0,036 | 0,035 | <b>0,037</b>     | 0,003                  | 1,00                                     | 0,50                                   |
| 10          | AES              | 0,032   | 0,035 | 0,041 | 0,041 | 0,040 | <b>0,038</b>     | 0,005                  | 1,33                                     | 0,67                                   |
| 6           | AES              | 0,047   | 0,050 | 0,033 | 0,030 | 0,034 | <b>0,039</b>     | 0,012                  | 1,67                                     | 0,83                                   |
| 12          | AES              | 0,044   | 0,040 | 0,037 | 0,042 | 0,039 | <b>0,040</b>     | 0,003                  | 2,00                                     | 1,00                                   |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 13 | 0,034                     | 0,003                  | 0,006                 | 0,002    |

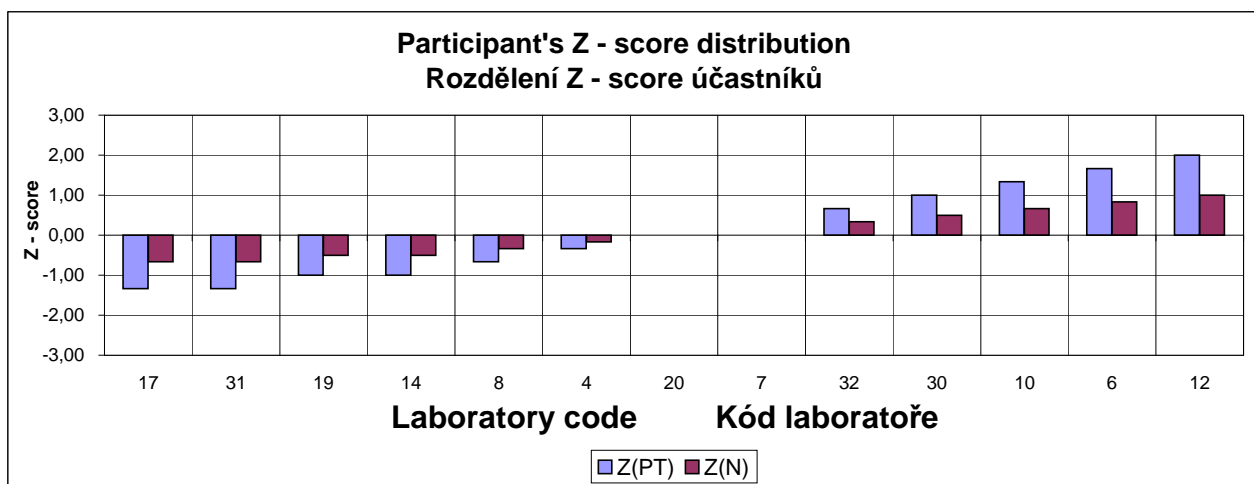


# PT 29/4A - W

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|--------|--------|--------|--------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     |                  |                        |  |  |
| 1           |                  | -   |        |        |        |        |                  |                        |  |  |
| 3           |                  | -   |        |        |        |        |                  |                        |  |  |
| 4           |                  | -   |        |        |        |        |                  |                        |  |  |
| 6           |                  | -   |        |        |        |        |                  |                        |  |  |
| 9           |                  | -   |        |        |        |        |                  |                        |  |  |
| 11          |                  | -   |        |        |        |        |                  |                        |  |  |
| 13          |                  | -   |        |        |        |        |                  |                        |  |  |
| 15          |                  | -   |        |        |        |        |                  |                        |  |  |
| 16          |                  | -   |        |        |        |        |                  |                        |  |  |
| 18          |                  | -   |        |        |        |        |                  |                        |  |  |
| 19          |                  | -   |        |        |        |        |                  |                        |  |  |
| 21          |                  | -   |        |        |        |        |                  |                        |  |  |
| 22          |                  | -   |        |        |        |        |                  |                        |  |  |
| 24          |                  | -   |        |        |        |        |                  |                        |  |  |
| 25          |                  | -   |        |        |        |        |                  |                        |  |  |
| 26          |                  | -   |        |        |        |        |                  |                        |  |  |
| 27          |                  | -   |        |        |        |        |                  |                        |  |  |
| 28          |                  | -   |        |        |        |        |                  |                        |  |  |
| 31          |                  | -   |        |        |        |        |                  |                        |  |  |
| 34          |                  | -   |        |        |        |        |                  |                        |  |  |
| 5           | AES              | 0,0100  | 0,0100 | 0,0082 | 0,0081 | 0,0088 | <b>0,0090</b>    | 0,0012                 | -1,76                                    | -1,38                                  |
| 23          | ICP              | 0,0110  | 0,0110 | 0,0111 | 0,0109 | 0,0108 | <b>0,0110</b>    | 0,0001                 | -1,07                                    | -0,84                                  |
| 14          | AES              | 0,0128  | 0,0110 | 0,0116 | 0,0107 | 0,0119 | <b>0,0116</b>    | 0,0010                 | -0,86                                    | -0,68                                  |
| 17          | ICP              | 0,0127  | 0,0130 | 0,0127 | 0,0107 | 0,0108 | <b>0,0120</b>    | 0,0014                 | -0,72                                    | -0,57                                  |
| 30          | AES              | 0,0100  | 0,0100 | 0,0100 | 0,0200 | 0,0100 | <b>0,0120</b>    | 0,0056                 | -0,72                                    | -0,57                                  |
| 7           | AES              | 0,0139  | 0,0138 | 0,0141 | 0,0138 | 0,0138 | <b>0,0139</b>    | 0,0002                 | -0,07                                    | -0,05                                  |
| 33          | XRF              | 0,0144  | 0,0141 | 0,0140 | 0,0147 | 0,0141 | <b>0,0143</b>    | 0,0004                 | 0,07                                     | 0,05                                   |
| 8           | AES              | 0,0160  | 0,0140 | 0,0140 | 0,0150 | 0,0140 | <b>0,0146</b>    | 0,0011                 | 0,17                                     | 0,14                                   |
| 2           | XRF              | 0,0130  | 0,0160 | 0,0150 | 0,0160 | 0,0150 | <b>0,0150</b>    | 0,0015                 | 0,31                                     | 0,24                                   |
| 32          | AES              | 0,0149  | 0,0138 | 0,0160 | 0,0157 | 0,0151 | <b>0,0151</b>    | 0,0011                 | 0,34                                     | 0,27                                   |
| 10          | AES              | 0,0160  | 0,0140 | 0,0140 | 0,0180 | 0,0140 | <b>0,0152</b>    | 0,0022                 | 0,38                                     | 0,30                                   |
| 12          | AES              | 0,0140  | 0,0160 | 0,0140 | 0,0170 | 0,0150 | <b>0,0152</b>    | 0,0016                 | 0,38                                     | 0,30                                   |
| 29          | AES              | 0,0170  | 0,0170 | 0,0170 | 0,0180 | 0,0170 | <b>0,0172</b>    | 0,0006                 | 1,07                                     | 0,84                                   |
| 20          | AES              | 0,0184  | 0,0209 | 0,0217 | 0,0223 | 0,0206 | <b>0,0208</b>    | 0,0018                 | 2,31                                     | 1,81                                   |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 14 | 0,0141                    | 0,0029                 | 0,0037                | 0,0017   |

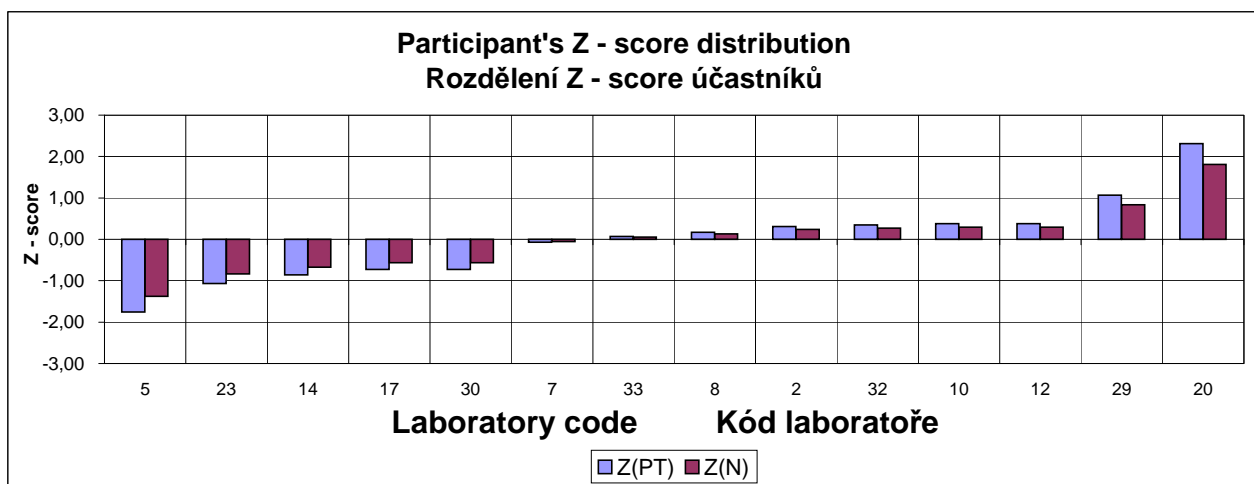



# PT 29/4A - V

## Results, statistical parameters and scoring


## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]        | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|-------|-------|-------|-------|--------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    | average      | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 3           |                  | -   |       |       |       |       |              |               |                       |                      |
| 15          |                  | -   |       |       |       |       |              |               |                       |                      |
| 16          |                  | -   |       |       |       |       |              |               |                       |                      |
| 21          |                  | -   |       |       |       |       |              |               |                       |                      |
| 22          |                  | -   |       |       |       |       |              |               |                       |                      |
| 23          |                  | -   |       |       |       |       |              |               |                       |                      |
| 24          |                  | -   |       |       |       |       |              |               |                       |                      |
| 25          |                  | -   |       |       |       |       |              |               |                       |                      |
| 26          |                  | -   |       |       |       |       |              |               |                       |                      |
| 28          |                  | -   |       |       |       |       |              |               |                       |                      |
| 34          |                  | -   |       |       |       |       |              |               |                       |                      |
| 30          | AES              | 0,330   | 0,330 | 0,340 | 0,340 | 0,340 | <b>0,336</b> | 0,007         | -1,87                 | -1,50                |
| 19          | AES              | 0,340   | 0,341 | 0,340 | 0,338 | 0,337 | <b>0,339</b> | 0,002         | -1,50                 | -1,20                |
| 6           | AES              | 0,344   | 0,336 | 0,338 | 0,343 | 0,338 | <b>0,340</b> | 0,004         | -1,37                 | -1,10                |
| 18          | AES              | 0,346   | 0,349 | 0,347 | 0,340 | 0,343 | <b>0,345</b> | 0,004         | -0,75                 | -0,60                |
| 8           | AES              | 0,347   | 0,345 | 0,348 | 0,349 | 0,347 | <b>0,347</b> | 0,002         | -0,50                 | -0,40                |
| 10          | AES              | 0,347   | 0,347 | 0,348 | 0,346 | 0,348 | <b>0,347</b> | 0,001         | -0,50                 | -0,40                |
| 12          | AES              | 0,347   | 0,349 | 0,348 | 0,348 | 0,347 | <b>0,348</b> | 0,001         | -0,38                 | -0,30                |
| 31          | AES              | 0,339   | 0,342 | 0,349 | 0,350 | 0,358 | <b>0,348</b> | 0,009         | -0,38                 | -0,30                |
| 9           | AES              | 0,347   | 0,350 | 0,349 | 0,351 | 0,349 | <b>0,349</b> | 0,002         | -0,25                 | -0,20                |
| 14          | AES              | 0,355   | 0,354 | 0,346 | 0,346 | 0,347 | <b>0,350</b> | 0,006         | -0,13                 | -0,10                |
| 11          | AES              | 0,352   | 0,350 | 0,348 | 0,350 | 0,349 | <b>0,350</b> | 0,002         | -0,13                 | -0,10                |
| 1           | AES              | 0,351   | 0,350 | 0,350 | 0,352 | 0,352 | <b>0,351</b> | 0,001         | 0,00                  | 0,00                 |
| 13          | AES              | 0,351   | 0,351 | 0,350 | 0,350 | 0,353 | <b>0,351</b> | 0,002         | 0,00                  | 0,00                 |
| 27          | XRF              | 0,350   | 0,351 | 0,350 | 0,352 | 0,350 | <b>0,351</b> | 0,001         | 0,00                  | 0,00                 |
| 29          | AES              | 0,353   | 0,355 | 0,355 | 0,352 | 0,352 | <b>0,353</b> | 0,002         | 0,25                  | 0,20                 |
| 32          | AES              | 0,357   | 0,356 | 0,355 | 0,354 | 0,355 | <b>0,355</b> | 0,001         | 0,50                  | 0,40                 |
| 5           | AES              | 0,350   | 0,354 | 0,360 | 0,357 | 0,355 | <b>0,355</b> | 0,005         | 0,50                  | 0,40                 |
| 7           | AES              | 0,354   | 0,358 | 0,359 | 0,359 | 0,357 | <b>0,357</b> | 0,003         | 0,75                  | 0,60                 |
| 17          | ICP              | 0,361   | 0,360 | 0,362 | 0,354 | 0,356 | <b>0,359</b> | 0,004         | 1,00                  | 0,80                 |
| 20          | AES              | 0,363   | 0,362 | 0,363 | 0,364 | 0,363 | <b>0,363</b> | 0,001         | 1,50                  | 1,20                 |
| 33          | XRF              | 0,366   | 0,364 | 0,364 | 0,365 | 0,363 | <b>0,364</b> | 0,001         | 1,63                  | 1,30                 |
| 2           | XRF              | 0,364   | 0,367 | 0,369 | 0,366 | 0,367 | <b>0,367</b> | 0,002         | 2,00                  | 1,60                 |
| 4*          | AES              | 0,399   | 0,381 | 0,391 |       |       | <b>0,390</b> | 0,022         | 4,88                  | 3,90                 |

\* - result excluded as outlier

\* - výsledek vyloučen jako odlehlý

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 22 | 0,351                     | 0,008                  | 0,010                 | 0,004    |

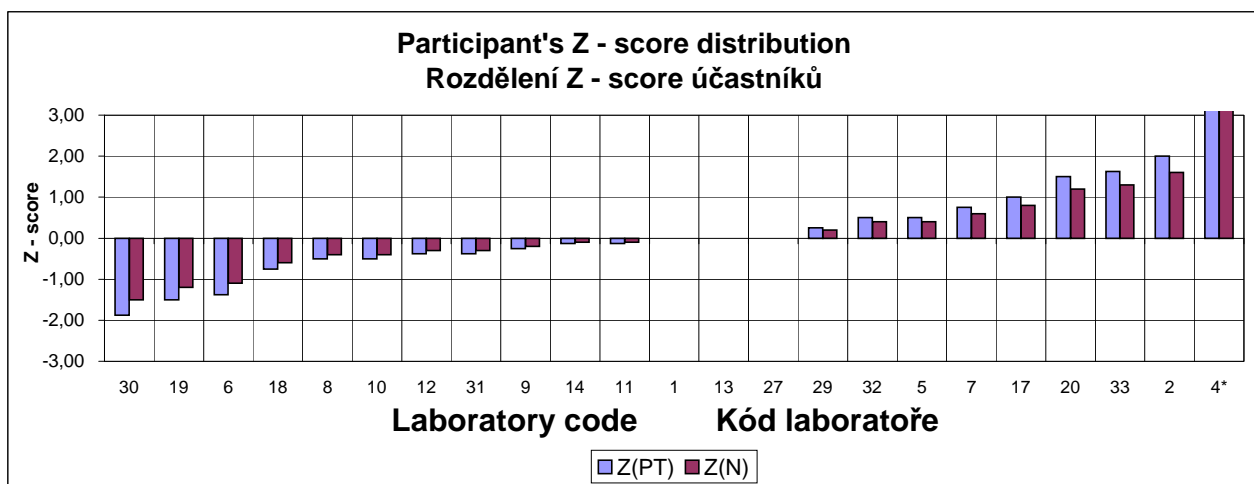


# PT 29/4A - Ti

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 3           |                  | -   |       |       |       |       |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 18          |                  | -   |       |       |       |       |                  |                        |  |  |
| 21          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 24          |                  | -   |       |       |       |       |                  |                        |  |  |
| 25          |                  | -   |       |       |       |       |                  |                        |  |  |
| 26          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 28          | ICP              | 0,066   | 0,066 | 0,070 | 0,067 | 0,066 | <b>0,067</b>     | 0,002                  | -2,17                                    | -1,86                                  |
| 31          | AES              | 0,077   | 0,068 | 0,073 | 0,064 | 0,068 | <b>0,070</b>     | 0,006                  | -1,67                                    | -1,43                                  |
| 23          | ICP              | 0,069   | 0,071 | 0,070 | 0,072 | 0,069 | <b>0,070</b>     | 0,002                  | -1,67                                    | -1,43                                  |
| 14          | AES              | 0,077   | 0,068 | 0,073 | 0,064 | 0,072 | <b>0,071</b>     | 0,006                  | -1,50                                    | -1,29                                  |
| 6           | AES              | 0,074   | 0,076 | 0,080 | 0,072 | 0,073 | <b>0,075</b>     | 0,004                  | -0,83                                    | -0,71                                  |
| 19          | AES              | 0,077   | 0,074 | 0,077 | 0,074 | 0,079 | <b>0,076</b>     | 0,003                  | -0,67                                    | -0,57                                  |
| 2           | XRF              | 0,071   | 0,076 | 0,083 | 0,074 | 0,082 | <b>0,077</b>     | 0,006                  | -0,50                                    | -0,43                                  |
| 20          | AES              | 0,078   | 0,080 | 0,078 | 0,078 | 0,078 | <b>0,078</b>     | 0,001                  | -0,33                                    | -0,29                                  |
| 11          | AES              | 0,077   | 0,084 | 0,076 | 0,077 | 0,076 | <b>0,078</b>     | 0,004                  | -0,33                                    | -0,29                                  |
| 8           | AES              | 0,075   | 0,077 | 0,077 | 0,080 | 0,083 | <b>0,078</b>     | 0,004                  | -0,33                                    | -0,29                                  |
| 1           | AES              | 0,083   | 0,077 | 0,071 | 0,087 | 0,077 | <b>0,079</b>     | 0,008                  | -0,17                                    | -0,14                                  |
| 13          | AES              | 0,087   | 0,078 | 0,080 | 0,075 | 0,082 | <b>0,080</b>     | 0,006                  | 0,00                                     | 0,00                                   |
| 17          | ICP              | 0,081   | 0,081 | 0,083 | 0,079 | 0,079 | <b>0,081</b>     | 0,002                  | 0,17                                     | 0,14                                   |
| 32          | AES              | 0,080   | 0,081 | 0,082 | 0,082 | 0,081 | <b>0,081</b>     | 0,001                  | 0,17                                     | 0,14                                   |
| 10          | AES              | 0,081   | 0,079 | 0,082 | 0,083 | 0,087 | <b>0,082</b>     | 0,004                  | 0,33                                     | 0,29                                   |
| 27          | XRF              | 0,081   | 0,082 | 0,082 | 0,083 | 0,082 | <b>0,082</b>     | 0,001                  | 0,33                                     | 0,29                                   |
| 7           | AES              | 0,080   | 0,082 | 0,080 | 0,088 | 0,081 | <b>0,082</b>     | 0,004                  | 0,33                                     | 0,29                                   |
| 9           | AES              | 0,077   | 0,087 | 0,077 | 0,085 | 0,083 | <b>0,082</b>     | 0,006                  | 0,33                                     | 0,29                                   |
| 4           | AES              | 0,081   | 0,079 | 0,090 |       |       | <b>0,083</b>     | 0,015                  | 0,50                                     | 0,43                                   |
| 30          | AES              | 0,087   | 0,078 | 0,093 | 0,084 | 0,082 | <b>0,085</b>     | 0,007                  | 0,83                                     | 0,71                                   |
| 29          | AES              | 0,087   | 0,094 | 0,084 | 0,084 | 0,083 | <b>0,086</b>     | 0,006                  | 1,00                                     | 0,86                                   |
| 5           | AES              | 0,087   | 0,091 | 0,089 | 0,081 | 0,093 | <b>0,088</b>     | 0,006                  | 1,33                                     | 1,14                                   |
| 33          | XRF              | 0,087   | 0,088 | 0,088 | 0,087 | 0,088 | <b>0,088</b>     | 0,001                  | 1,33                                     | 1,14                                   |
| 12          | AES              | 0,090   | 0,091 | 0,084 | 0,094 | 0,089 | <b>0,090</b>     | 0,005                  | 1,67                                     | 1,43                                   |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 24 | 0,080                     | 0,006                  | 0,007                 | 0,003    |

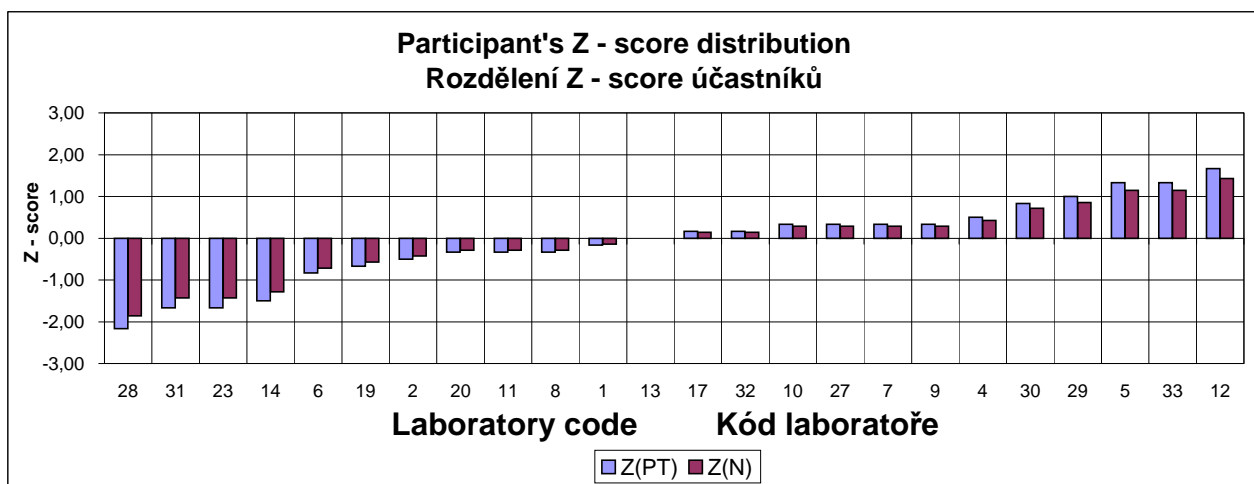


# PT 29/4A - Co

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 3           |                  | -   |       |       |       |       |                  |                        |  |  |
| 9           |                  | -   |       |       |       |       |                  |                        |  |  |
| 11          |                  | -   |       |       |       |       |                  |                        |  |  |
| 13          |                  | -   |       |       |       |       |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 21          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 24          |                  | -   |       |       |       |       |                  |                        |  |  |
| 25          |                  | -   |       |       |       |       |                  |                        |  |  |
| 26          |                  | -   |       |       |       |       |                  |                        |  |  |
| 27          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 33          | XRF              | 0,053   | 0,053 | 0,052 | 0,052 | 0,052 | <b>0,052</b>     | 0,001                  | -2,33                                    | -1,84                                  |
| 23          | ICP              | 0,051   | 0,053 | 0,054 | 0,053 | 0,053 | <b>0,053</b>     | 0,001                  | -2,00                                    | -1,58                                  |
| 19          | AES              | 0,060   | 0,060 | 0,061 | 0,052 | 0,049 | <b>0,056</b>     | 0,007                  | -1,00                                    | -0,79                                  |
| 5           | AES              | 0,059   | 0,054 | 0,057 | 0,057 | 0,054 | <b>0,056</b>     | 0,003                  | -1,00                                    | -0,79                                  |
| 1           | AES              | 0,057   | 0,057 | 0,057 | 0,057 | 0,057 | <b>0,057</b>     | 0,000                  | -0,67                                    | -0,53                                  |
| 2           | XRF              | 0,057   | 0,058 | 0,056 | 0,057 | 0,058 | <b>0,057</b>     | 0,001                  | -0,67                                    | -0,53                                  |
| 29          | AES              | 0,057   | 0,057 | 0,057 | 0,057 | 0,057 | <b>0,057</b>     | 0,000                  | -0,67                                    | -0,53                                  |
| 32          | AES              | 0,058   | 0,058 | 0,057 | 0,057 | 0,058 | <b>0,058</b>     | 0,001                  | -0,33                                    | -0,26                                  |
| 8           | AES              | 0,059   | 0,059 | 0,059 | 0,059 | 0,059 | <b>0,059</b>     | 0,000                  | 0,00                                     | 0,00                                   |
| 17          | ICP              | 0,059   | 0,058 | 0,059 | 0,059 | 0,058 | <b>0,059</b>     | 0,001                  | 0,00                                     | 0,00                                   |
| 10          | AES              | 0,061   | 0,059 | 0,059 | 0,061 | 0,059 | <b>0,060</b>     | 0,001                  | 0,33                                     | 0,26                                   |
| 12          | AES              | 0,061   | 0,061 | 0,059 | 0,059 | 0,059 | <b>0,060</b>     | 0,001                  | 0,33                                     | 0,26                                   |
| 7           | AES              | 0,060   | 0,060 | 0,060 | 0,060 | 0,060 | <b>0,060</b>     | 0,000                  | 0,33                                     | 0,26                                   |
| 30          | AES              | 0,060   | 0,060 | 0,060 | 0,060 | 0,060 | <b>0,060</b>     | 0,000                  | 0,33                                     | 0,26                                   |
| 4           | AES              | 0,062   | 0,060 | 0,062 |       |       | <b>0,061</b>     | 0,003                  | 0,67                                     | 0,53                                   |
| 28          | ICP              | 0,062   | 0,063 | 0,063 | 0,063 | 0,062 | <b>0,062</b>     | 0,001                  | 1,00                                     | 0,79                                   |
| 20          | AES              | 0,062   | 0,062 | 0,062 | 0,063 | 0,063 | <b>0,062</b>     | 0,001                  | 1,00                                     | 0,79                                   |
| 14          | AES              | 0,060   | 0,063 | 0,061 | 0,065 | 0,068 | <b>0,063</b>     | 0,004                  | 1,33                                     | 1,05                                   |
| 31          | AES              | 0,060   | 0,063 | 0,061 | 0,065 | 0,068 | <b>0,063</b>     | 0,004                  | 1,33                                     | 1,05                                   |
| 6           | AES              | 0,063   | 0,063 | 0,065 | 0,065 | 0,063 | <b>0,064</b>     | 0,001                  | 1,67                                     | 1,32                                   |
| 18          | AES              | 0,063   | 0,066 | 0,064 | 0,067 | 0,064 | <b>0,065</b>     | 0,002                  | 2,00                                     | 1,58                                   |

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 21 | 0,059                     | 0,003                  | 0,004                 | 0,001    |

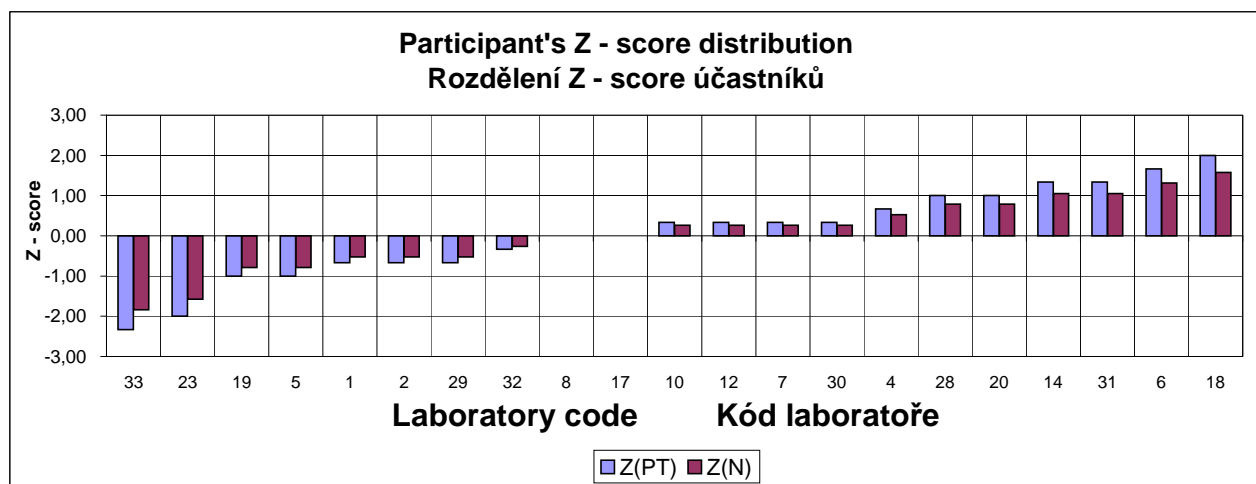


# PT 29/4A - As

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|--------|--------|--------|--------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     |                  |                        |  |  |
| 1           |                  | -   |        |        |        |        |                  |                        |  |  |
| 2           |                  | -   |        |        |        |        |                  |                        |  |  |
| 3           |                  | -   |        |        |        |        |                  |                        |  |  |
| 4           |                  | -   |        |        |        |        |                  |                        |  |  |
| 5           |                  | -   |        |        |        |        |                  |                        |  |  |
| 6           |                  | -   |        |        |        |        |                  |                        |  |  |
| 9           |                  | -   |        |        |        |        |                  |                        |  |  |
| 11          |                  | -   |        |        |        |        |                  |                        |  |  |
| 13          |                  | -   |        |        |        |        |                  |                        |  |  |
| 14          |                  | -   |        |        |        |        |                  |                        |  |  |
| 15          |                  | -   |        |        |        |        |                  |                        |  |  |
| 16          |                  | -   |        |        |        |        |                  |                        |  |  |
| 18          |                  | -   |        |        |        |        |                  |                        |  |  |
| 21          |                  | -   |        |        |        |        |                  |                        |  |  |
| 22          |                  | -   |        |        |        |        |                  |                        |  |  |
| 24          |                  | -   |        |        |        |        |                  |                        |  |  |
| 25          |                  | -   |        |        |        |        |                  |                        |  |  |
| 26          |                  | -   |        |        |        |        |                  |                        |  |  |
| 28          |                  | -   |        |        |        |        |                  |                        |  |  |
| 31          |                  | -   |        |        |        |        |                  |                        |  |  |
| 34          |                  | -   |        |        |        |        |                  |                        |  |  |
| 30          | AES              | 0,0050  | 0,0060 | 0,0060 | 0,0060 | 0,0050 | <b>0,0056</b>    | 0,0007                 | -1,83                                    | -1,05                                  |
| 19          | AES              | 0,0060  | 0,0065 | 0,0063 | 0,0067 | 0,0062 | <b>0,0063</b>    | 0,0003                 | -1,25                                    | -0,71                                  |
| 17          | ICP              | 0,0067  | 0,0070 | 0,0071 | 0,0069 | 0,0071 | <b>0,0070</b>    | 0,0002                 | -0,67                                    | -0,38                                  |
| 23          | ICP              | 0,0070  | 0,0080 | 0,0070 | 0,0080 | 0,0070 | <b>0,0074</b>    | 0,0007                 | -0,33                                    | -0,19                                  |
| 20          | AES              | 0,0086  | 0,0068 | 0,0082 | 0,0073 | 0,0079 | <b>0,0078</b>    | 0,0009                 | 0,00                                     | 0,00                                   |
| 7           | AES              | 0,0077  | 0,0079 | 0,0080 | 0,0077 | 0,0077 | <b>0,0078</b>    | 0,0002                 | 0,00                                     | 0,00                                   |
| 32          | AES              | 0,0081  | 0,0076 | 0,0079 | 0,0081 | 0,0083 | <b>0,0080</b>    | 0,0003                 | 0,17                                     | 0,10                                   |
| 33          | XRF              | 0,0081  | 0,0082 | 0,0076 | 0,0079 | 0,0080 | <b>0,0080</b>    | 0,0003                 | 0,17                                     | 0,10                                   |
| 8           | AES              | 0,0080  | 0,0080 | 0,0080 | 0,0080 | 0,0080 | <b>0,0080</b>    | 0,0000                 | 0,17                                     | 0,10                                   |
| 12          | AES              | 0,0080  | 0,0080 | 0,0080 | 0,0090 | 0,0080 | <b>0,0082</b>    | 0,0006                 | 0,33                                     | 0,19                                   |
| 10          | AES              | 0,0080  | 0,0080 | 0,0090 | 0,0080 | 0,0090 | <b>0,0084</b>    | 0,0007                 | 0,50                                     | 0,29                                   |
| 27          | XRF              | 0,0096  | 0,0078 | 0,0119 | 0,0069 | 0,0110 | <b>0,0094</b>    | 0,0026                 | 1,33                                     | 0,76                                   |
| 29          | AES              | 0,0100  | 0,0100 | 0,0100 | 0,0100 | 0,0100 | <b>0,0100</b>    | 0,0000                 | 1,83                                     | 1,05                                   |

| n  | $\hat{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 13 | 0,0078                    | 0,0012                 | 0,0021                | 0,0007   |

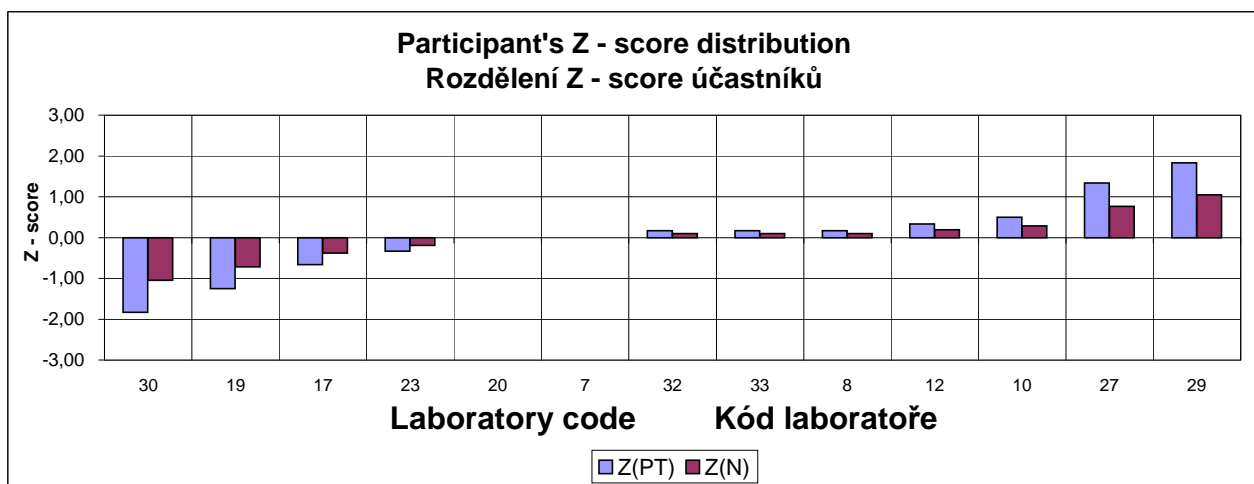

# PT 29/4A - Sn

## Results, statistical parameters and scoring


## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|--------|--------|--------|--------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     |                  |                        |  |  |
| 1           |                  | -   |        |        |        |        |                  |                        |  |  |
| 3           |                  | -   |        |        |        |        |                  |                        |  |  |
| 15          |                  | -   |        |        |        |        |                  |                        |  |  |
| 16          |                  | -   |        |        |        |        |                  |                        |  |  |
| 21          |                  | -   |        |        |        |        |                  |                        |  |  |
| 22          |                  | -   |        |        |        |        |                  |                        |  |  |
| 23          |                  | -   |        |        |        |        |                  |                        |  |  |
| 24          |                  | -   |        |        |        |        |                  |                        |  |  |
| 25          |                  | -   |        |        |        |        |                  |                        |  |  |
| 26          |                  | -   |        |        |        |        |                  |                        |  |  |
| 27          |                  | -   |        |        |        |        |                  |                        |  |  |
| 29          |                  | -   |        |        |        |        |                  |                        |  |  |
| 34          |                  | -   |        |        |        |        |                  |                        |  |  |
| 28          | ICP              | 0,0212  | 0,0210 | 0,0200 | 0,0191 | 0,0209 | <b>0,0204</b>    | 0,0011                 | -2,14                                    | -1,11                                  |
| 2           | XRF              | 0,0223  | 0,0191 | 0,0211 | 0,0214 | 0,0200 | <b>0,0208</b>    | 0,0015                 | -1,86                                    | -0,96                                  |
| 17          | ICP              | 0,0220  | 0,0210 | 0,0220 | 0,0210 | 0,0190 | <b>0,0210</b>    | 0,0015                 | -1,71                                    | -0,89                                  |
| 18          | AES              | 0,0224  | 0,0223 | 0,0221 | 0,0244 | 0,0233 | <b>0,0229</b>    | 0,0012                 | -0,36                                    | -0,19                                  |
| 32          | AES              | 0,0234  | 0,0228 | 0,0227 | 0,0234 | 0,0229 | <b>0,0230</b>    | 0,0004                 | -0,29                                    | -0,15                                  |
| 19          | AES              | 0,0234  | 0,0237 | 0,0240 | 0,0227 | 0,0224 | <b>0,0232</b>    | 0,0008                 | -0,14                                    | -0,07                                  |
| 5           | AES              | 0,0230  | 0,0230 | 0,0240 | 0,0240 | 0,0220 | <b>0,0232</b>    | 0,0010                 | -0,14                                    | -0,07                                  |
| 13          | AES              | 0,0230  | 0,0230 | 0,0228 | 0,0235 | 0,0237 | <b>0,0232</b>    | 0,0005                 | -0,14                                    | -0,07                                  |
| 11          | AES              | 0,0237  | 0,0230 | 0,0229 | 0,0233 | 0,0236 | <b>0,0233</b>    | 0,0004                 | -0,07                                    | -0,04                                  |
| 7           | AES              | 0,0232  | 0,0233 | 0,0237 | 0,0230 | 0,0231 | <b>0,0233</b>    | 0,0003                 | -0,07                                    | -0,04                                  |
| 30          | AES              | 0,0230  | 0,0230 | 0,0240 | 0,0240 | 0,0230 | <b>0,0234</b>    | 0,0007                 | 0,00                                     | 0,00                                   |
| 8           | AES              | 0,0230  | 0,0230 | 0,0240 | 0,0240 | 0,0240 | <b>0,0236</b>    | 0,0007                 | 0,14                                     | 0,07                                   |
| 33          | XRF              | 0,0237  | 0,0231 | 0,0233 | 0,0240 | 0,0242 | <b>0,0237</b>    | 0,0006                 | 0,21                                     | 0,11                                   |
| 9           | AES              | 0,0229  | 0,0238 | 0,0238 | 0,0241 | 0,0245 | <b>0,0238</b>    | 0,0007                 | 0,29                                     | 0,15                                   |
| 10          | AES              | 0,0240  | 0,0240 | 0,0240 | 0,0240 | 0,0240 | <b>0,0240</b>    | 0,0000                 | 0,43                                     | 0,22                                   |
| 12          | AES              | 0,0240  | 0,0240 | 0,0240 | 0,0250 | 0,0240 | <b>0,0242</b>    | 0,0006                 | 0,57                                     | 0,30                                   |
| 6           | AES              | 0,0241  | 0,0245 | 0,0249 | 0,0238 | 0,0242 | <b>0,0243</b>    | 0,0005                 | 0,64                                     | 0,33                                   |
| 14          | AES              | 0,0276  | 0,0243 | 0,0258 | 0,0252 | 0,0242 | <b>0,0254</b>    | 0,0017                 | 1,43                                     | 0,74                                   |
| 31          | AES              | 0,0252  | 0,0253 | 0,0266 | 0,0236 | 0,0262 | <b>0,0254</b>    | 0,0014                 | 1,43                                     | 0,74                                   |
| 20          | AES              | 0,0254  | 0,0253 | 0,0264 | 0,0262 | 0,0261 | <b>0,0259</b>    | 0,0006                 | 1,79                                     | 0,93                                   |
| 4*          | AES              | 0,0360  | 0,0340 | 0,0340 |        |        | <b>0,0347</b>    | 0,0029                 | 8,07                                     | 4,19                                   |

\* - result excluded as outlier

\* - výsledek vyloučen jako odlehlý

| n  | $\bar{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 20 | 0,0234                    | 0,0014                 | 0,0027                | 0,0007   |

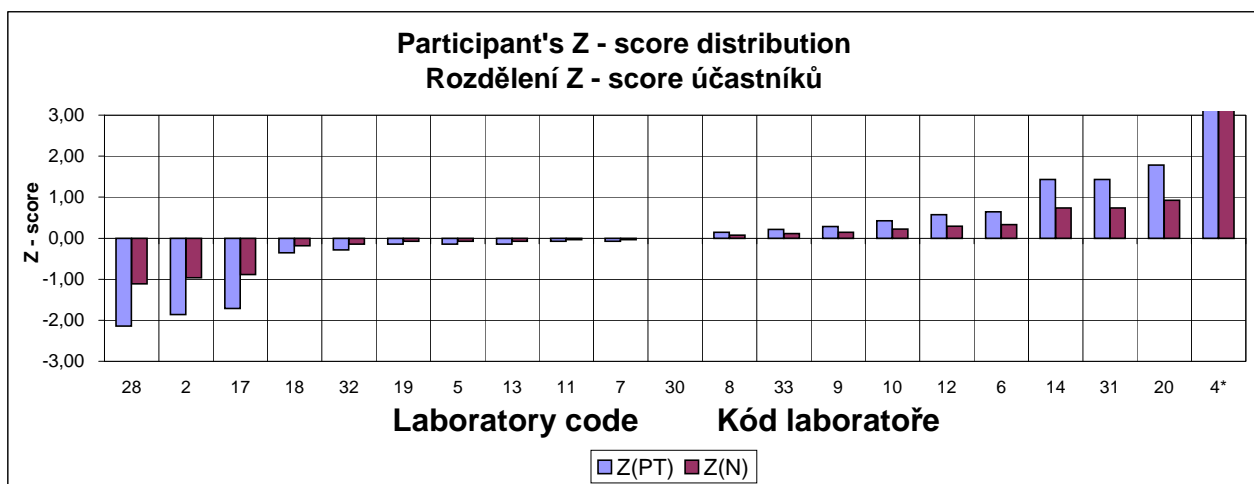


# PT 29/4A - Zn

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]         | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|--------|--------|--------|--------|---------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     | average       | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 3           |                  | -   |        |        |        |        |               |               |                       |                      |
| 4           |                  | -   |        |        |        |        |               |               |                       |                      |
| 9           |                  | -   |        |        |        |        |               |               |                       |                      |
| 11          |                  | -   |        |        |        |        |               |               |                       |                      |
| 13          |                  | -   |        |        |        |        |               |               |                       |                      |
| 15          |                  | -   |        |        |        |        |               |               |                       |                      |
| 16          |                  | -   |        |        |        |        |               |               |                       |                      |
| 18          |                  | -   |        |        |        |        |               |               |                       |                      |
| 21          |                  | -   |        |        |        |        |               |               |                       |                      |
| 22          |                  | -   |        |        |        |        |               |               |                       |                      |
| 24          |                  | -   |        |        |        |        |               |               |                       |                      |
| 25          |                  | -   |        |        |        |        |               |               |                       |                      |
| 26          |                  | -   |        |        |        |        |               |               |                       |                      |
| 28          |                  | -   |        |        |        |        |               |               |                       |                      |
| 29          |                  | -   |        |        |        |        |               |               |                       |                      |
| 34          |                  | -   |        |        |        |        |               |               |                       |                      |
| 19          | AES              | 0,0164  | 0,0170 | 0,0150 | 0,0167 | 0,0145 | <b>0,0159</b> | 0,0014        | -1,52                 | -1,25                |
| 14          | AES              | 0,0152  | 0,0152 | 0,0173 | 0,0149 | 0,0177 | <b>0,0161</b> | 0,0016        | -1,43                 | -1,18                |
| 8           | AES              | 0,0170  | 0,0170 | 0,0170 | 0,0170 | 0,0170 | <b>0,0170</b> | 0,0000        | -1,04                 | -0,86                |
| 12          | AES              | 0,0170  | 0,0170 | 0,0170 | 0,0170 | 0,0170 | <b>0,0170</b> | 0,0000        | -1,04                 | -0,86                |
| 10          | AES              | 0,0170  | 0,0170 | 0,0180 | 0,0170 | 0,0180 | <b>0,0174</b> | 0,0007        | -0,87                 | -0,71                |
| 31          | AES              | 0,0175  | 0,0174 | 0,0180 | 0,0178 | 0,0186 | <b>0,0179</b> | 0,0006        | -0,65                 | -0,54                |
| 32          | AES              | 0,0192  | 0,0179 | 0,0185 | 0,0192 | 0,0195 | <b>0,0189</b> | 0,0008        | -0,22                 | -0,18                |
| 33          | XRF              | 0,0192  | 0,0188 | 0,0189 | 0,0191 | 0,0191 | <b>0,0190</b> | 0,0002        | -0,17                 | -0,14                |
| 2           | XRF              | 0,0193  | 0,0196 | 0,0197 | 0,0190 | 0,0193 | <b>0,0194</b> | 0,0003        | 0,00                  | 0,00                 |
| 1           | AES              | 0,0192  | 0,0193 | 0,0194 | 0,0198 | 0,0199 | <b>0,0195</b> | 0,0004        | 0,04                  | 0,04                 |
| 5           | AES              | 0,0190  | 0,0190 | 0,0210 | 0,0200 | 0,0200 | <b>0,0198</b> | 0,0010        | 0,17                  | 0,14                 |
| 6           | AES              | 0,0202  | 0,0227 | 0,0192 | 0,0190 | 0,0188 | <b>0,0200</b> | 0,0020        | 0,26                  | 0,21                 |
| 17          | ICP              | 0,0195  | 0,0189 | 0,0192 | 0,0225 | 0,0225 | <b>0,0205</b> | 0,0023        | 0,48                  | 0,39                 |
| 23          | ICP              | 0,0230  | 0,0210 | 0,0210 | 0,0200 | 0,0230 | <b>0,0216</b> | 0,0017        | 0,96                  | 0,79                 |
| 7           | AES              | 0,0212  | 0,0219 | 0,0222 | 0,0216 | 0,0214 | <b>0,0217</b> | 0,0005        | 1,00                  | 0,82                 |
| 30          | AES              | 0,0220  | 0,0216 | 0,0226 | 0,0234 | 0,0214 | <b>0,0222</b> | 0,0010        | 1,22                  | 1,00                 |
| 27          | XRF              | 0,0230  | 0,0220 | 0,0234 | 0,0231 | 0,0217 | <b>0,0226</b> | 0,0009        | 1,39                  | 1,14                 |
| 20          | AES              | 0,0229  | 0,0232 | 0,0233 | 0,0238 | 0,0238 | <b>0,0234</b> | 0,0005        | 1,74                  | 1,43                 |

| n  | $\hat{X} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 18 | 0,0194                    | 0,0023                 | 0,0028                | 0,0011   |

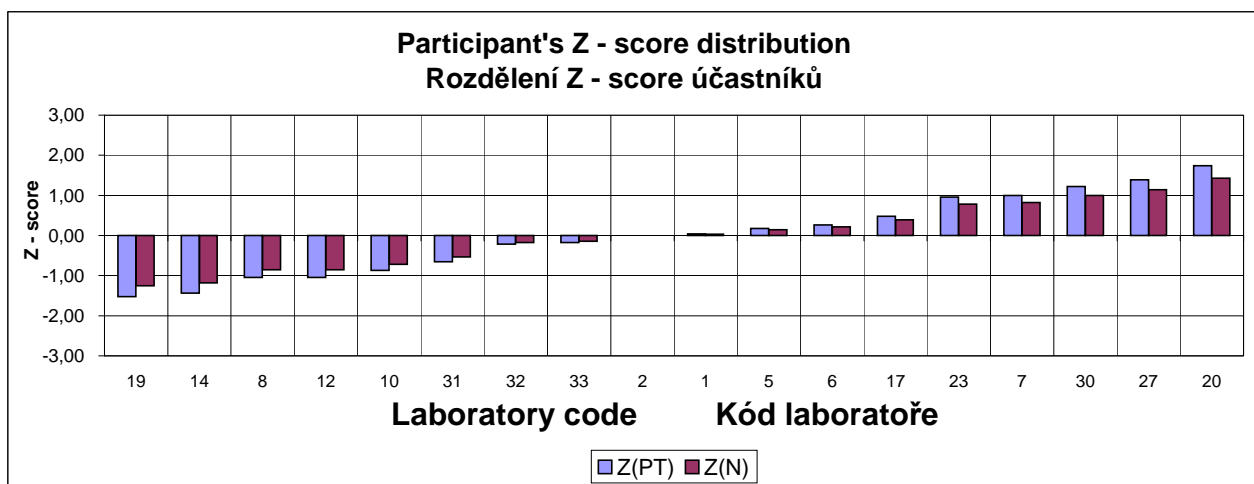


PT 29/4A - Zr

Results, statistical parameters and scoring

Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |       |       |       |       | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|-------|-------|-------|-------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.    | 3.    | 4.    | 5.    |                  |                        |  |  |
| 1           |                  | -   |       |       |       |       |                  |                        |  |  |
| 2           |                  | -   |       |       |       |       |                  |                        |  |  |
| 3           |                  | -   |       |       |       |       |                  |                        |  |  |
| 4           |                  | -   |       |       |       |       |                  |                        |  |  |
| 5           |                  | -   |       |       |       |       |                  |                        |  |  |
| 9           |                  | -   |       |       |       |       |                  |                        |  |  |
| 11          |                  | -   |       |       |       |       |                  |                        |  |  |
| 13          |                  | -   |       |       |       |       |                  |                        |  |  |
| 14          |                  | -   |       |       |       |       |                  |                        |  |  |
| 15          |                  | -   |       |       |       |       |                  |                        |  |  |
| 16          |                  | -   |       |       |       |       |                  |                        |  |  |
| 17          |                  | -   |       |       |       |       |                  |                        |  |  |
| 18          |                  | -   |       |       |       |       |                  |                        |  |  |
| 21          |                  | -   |       |       |       |       |                  |                        |  |  |
| 22          |                  | -   |       |       |       |       |                  |                        |  |  |
| 23          |                  | -   |       |       |       |       |                  |                        |  |  |
| 24          |                  | -   |       |       |       |       |                  |                        |  |  |
| 25          |                  | -   |       |       |       |       |                  |                        |  |  |
| 26          |                  | -   |       |       |       |       |                  |                        |  |  |
| 27          |                  | -   |       |       |       |       |                  |                        |  |  |
| 28          |                  | -   |       |       |       |       |                  |                        |  |  |
| 29          |                  | -   |       |       |       |       |                  |                        |  |  |
| 30          |                  | -   |       |       |       |       |                  |                        |  |  |
| 31          |                  | -   |       |       |       |       |                  |                        |  |  |
| 34          |                  | -   |       |       |       |       |                  |                        |  |  |
| 20          | AES              | 0,039   | 0,039 | 0,040 | 0,040 | 0,039 | <b>0,039</b>     | 0,001                  | -1,50                                    | -1,30                                  |
| 8           | AES              | 0,040   | 0,040 | 0,040 | 0,040 | 0,041 | <b>0,040</b>     | 0,001                  | -1,00                                    | -0,87                                  |
| 19          | AES              | 0,041   | 0,041 | 0,043 | 0,040 | 0,041 | <b>0,041</b>     | 0,001                  | -0,50                                    | -0,43                                  |
| 6           | AES              | 0,041   | 0,041 | 0,041 | 0,040 | 0,040 | <b>0,041</b>     | 0,001                  | -0,50                                    | -0,43                                  |
| 12          | AES              | 0,042   | 0,043 | 0,041 | 0,042 | 0,042 | <b>0,042</b>     | 0,001                  | 0,00                                     | 0,00                                   |
| 10          | AES              | 0,041   | 0,041 | 0,042 | 0,042 | 0,042 | <b>0,042</b>     | 0,001                  | 0,00                                     | 0,00                                   |
| 32          | AES              | 0,041   | 0,042 | 0,043 | 0,043 | 0,041 | <b>0,042</b>     | 0,001                  | 0,00                                     | 0,00                                   |
| 7           | AES              | 0,042   | 0,043 | 0,043 | 0,044 | 0,042 | <b>0,043</b>     | 0,001                  | 0,50                                     | 0,43                                   |
| 33          | XRF              | 0,044   | 0,044 | 0,043 | 0,043 | 0,044 | <b>0,044</b>     | 0,001                  | 1,00                                     | 0,87                                   |

| n | $\hat{x} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|---|---------------------------|------------------------|-----------------------|----------|
| 9 | 0,042                     | 0,002                  | 0,002                 | 0,002    |

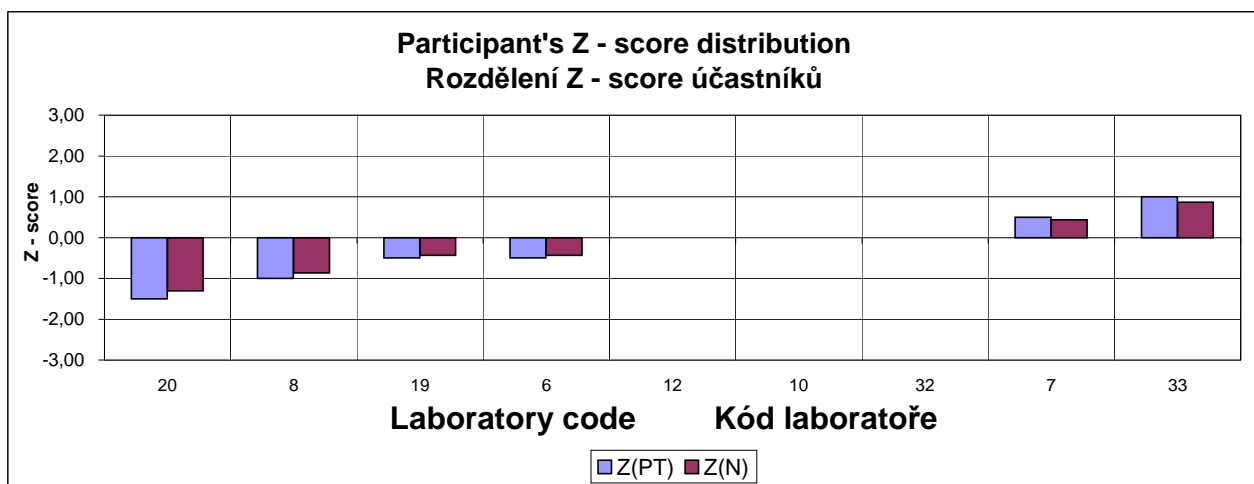


# PT 29/4A - B

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]<br>average | u [%]<br>repeatability | Z <sub>PT</sub><br>Z-score <sub>PT</sub> | Z <sub>N</sub><br>Z-score <sub>N</sub> |
|-------------|------------------|---|--------|--------|--------|--------|------------------|------------------------|--|--|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     |                  |                        |  |  |
| 1           |                  | -   |        |        |        |        |                  |                        |  |  |
| 2           |                  | -   |        |        |        |        |                  |                        |  |  |
| 3           |                  | -   |        |        |        |        |                  |                        |  |  |
| 4           |                  | -   |        |        |        |        |                  |                        |  |  |
| 9           |                  | -   |        |        |        |        |                  |                        |  |  |
| 11          |                  | -   |        |        |        |        |                  |                        |  |  |
| 13          |                  | -   |        |        |        |        |                  |                        |  |  |
| 15          |                  | -   |        |        |        |        |                  |                        |  |  |
| 16          |                  | -   |        |        |        |        |                  |                        |  |  |
| 17          |                  | -   |        |        |        |        |                  |                        |  |  |
| 18          |                  | -   |        |        |        |        |                  |                        |  |  |
| 19          |                  | -   |        |        |        |        |                  |                        |  |  |
| 21          |                  | -   |        |        |        |        |                  |                        |  |  |
| 22          |                  | -   |        |        |        |        |                  |                        |  |  |
| 23          |                  | -   |        |        |        |        |                  |                        |  |  |
| 24          |                  | -   |        |        |        |        |                  |                        |  |  |
| 25          |                  | -   |        |        |        |        |                  |                        |  |  |
| 26          |                  | -   |        |        |        |        |                  |                        |  |  |
| 27          |                  | -   |        |        |        |        |                  |                        |  |  |
| 28          |                  | -   |        |        |        |        |                  |                        |  |  |
| 33          |                  | -   |        |        |        |        |                  |                        |  |  |
| 34          |                  | -   |        |        |        |        |                  |                        |  |  |
| 32          | AES              | 0,0032  | 0,0030 | 0,0034 | 0,0034 | 0,0030 | <b>0,0032</b>    | 0,0002                 | -1,33                                    | -0,80                                  |
| 12          | AES              | 0,0035  | 0,0034 | 0,0034 | 0,0035 | 0,0034 | <b>0,0034</b>    | 0,0001                 | -0,67                                    | -0,40                                  |
| 5           | AES              | 0,0034  | 0,0032 | 0,0033 | 0,0032 | 0,0041 | <b>0,0034</b>    | 0,0005                 | -0,67                                    | -0,40                                  |
| 7           | AES              | 0,0034  | 0,0034 | 0,0034 | 0,0034 | 0,0034 | <b>0,0034</b>    | 0,0000                 | -0,67                                    | -0,40                                  |
| 10          | AES              | 0,0034  | 0,0033 | 0,0035 | 0,0035 | 0,0034 | <b>0,0034</b>    | 0,0001                 | -0,67                                    | -0,40                                  |
| 8           | AES              | 0,0033  | 0,0034 | 0,0034 | 0,0034 | 0,0034 | <b>0,0034</b>    | 0,0001                 | -0,67                                    | -0,40                                  |
| 6           | AES              | 0,0035  | 0,0033 | 0,0037 | 0,0034 | 0,0034 | <b>0,0035</b>    | 0,0002                 | -0,33                                    | -0,20                                  |
| 30          | AES              | 0,0036  | 0,0036 | 0,0037 | 0,0038 | 0,0037 | <b>0,0037</b>    | 0,0001                 | 0,33                                     | 0,20                                   |
| 14          | AES              | 0,0042  | 0,0039 | 0,0039 | 0,0037 | 0,0039 | <b>0,0039</b>    | 0,0002                 | 1,00                                     | 0,60                                   |
| 20          | AES              | 0,0040  | 0,0040 | 0,0040 | 0,0040 | 0,0039 | <b>0,0040</b>    | 0,0001                 | 1,33                                     | 0,80                                   |
| 31          | AES              | 0,0038  | 0,0038 | 0,0047 | 0,0040 | 0,0044 | <b>0,0041</b>    | 0,0005                 | 1,67                                     | 1,00                                   |
| 29          | AES              | 0,0042  | 0,0042 | 0,0042 | 0,0042 | 0,0042 | <b>0,0042</b>    | 0,0000                 | 2,00                                     | 1,20                                   |

| n  | $\hat{X} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 12 | 0,0036                    | 0,0003                 | 0,0005                | 0,0002   |

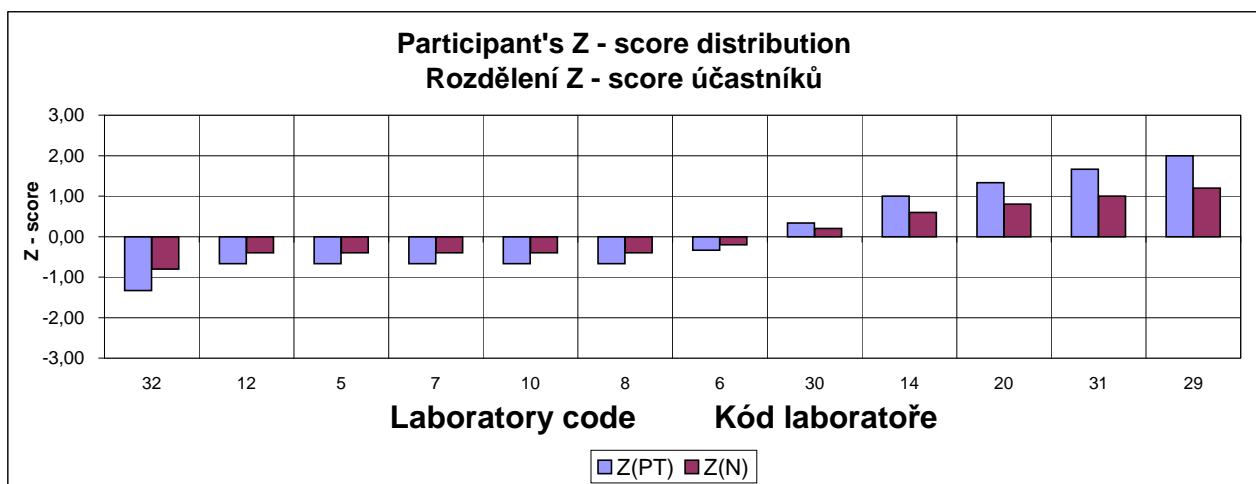



# PT 29/4A - Nb

## Results, statistical parameters and scoring

## Výsledky, statistické parametry a scoring

| Code<br>Kód | Method<br>Metoda | Individual results % [wt. %], Jednotlivé výsledky [hm. %] |        |        |        |        | x [%]         | u [%]         | Z <sub>PT</sub>       | Z <sub>N</sub>       |
|-------------|------------------|---|--------|--------|--------|--------|---------------|---------------|-----------------------|----------------------|
|             |                  | 1.  | 2.     | 3.     | 4.     | 5.     | average       | repeatability | Z-score <sub>PT</sub> | Z-score <sub>N</sub> |
| 1           |                  | -   |        |        |        |        |               |               |                       |                      |
| 3           |                  | -   |        |        |        |        |               |               |                       |                      |
| 14          |                  | -   |        |        |        |        |               |               |                       |                      |
| 15          |                  | -   |        |        |        |        |               |               |                       |                      |
| 16          |                  | -   |        |        |        |        |               |               |                       |                      |
| 18          |                  | -   |        |        |        |        |               |               |                       |                      |
| 21          |                  | -   |        |        |        |        |               |               |                       |                      |
| 22          |                  | -   |        |        |        |        |               |               |                       |                      |
| 23          |                  | -   |        |        |        |        |               |               |                       |                      |
| 24          |                  | -   |        |        |        |        |               |               |                       |                      |
| 25          |                  | -   |        |        |        |        |               |               |                       |                      |
| 26          |                  | -   |        |        |        |        |               |               |                       |                      |
| 27          |                  | -   |        |        |        |        |               |               |                       |                      |
| 28          |                  | -   |        |        |        |        |               |               |                       |                      |
| 30          |                  | -   |        |        |        |        |               |               |                       |                      |
| 31          |                  | -   |        |        |        |        |               |               |                       |                      |
| 34          |                  | -   |        |        |        |        |               |               |                       |                      |
| 17          | ICP              | 0,0077  | 0,0076 | 0,0078 | 0,0076 | 0,0078 | <b>0,0077</b> | 0,0001        | -1,69                 | -1,22                |
| 2           | XRF              | 0,0082  | 0,0084 | 0,0081 | 0,0084 | 0,0083 | <b>0,0083</b> | 0,0002        | -1,23                 | -0,89                |
| 8           | AES              | 0,0090  | 0,0090 | 0,0090 | 0,0090 | 0,0090 | <b>0,0090</b> | 0,0000        | -0,69                 | -0,50                |
| 10          | AES              | 0,0090  | 0,0090 | 0,0090 | 0,0090 | 0,0090 | <b>0,0090</b> | 0,0000        | -0,69                 | -0,50                |
| 12          | AES              | 0,0090  | 0,0090 | 0,0090 | 0,0090 | 0,0090 | <b>0,0090</b> | 0,0000        | -0,69                 | -0,50                |
| 11          | AES              | 0,0110  | 0,0090 | 0,0090 | 0,0090 | 0,0090 | <b>0,0094</b> | 0,0011        | -0,38                 | -0,28                |
| 19          | AES              | 0,0092  | 0,0093 | 0,0100 | 0,0091 | 0,0092 | <b>0,0094</b> | 0,0005        | -0,38                 | -0,28                |
| 20          | AES              | 0,0096  | 0,0100 | 0,0093 | 0,0102 | 0,0099 | <b>0,0098</b> | 0,0004        | -0,08                 | -0,06                |
| 5           | AES              | 0,0098  | 0,0097 | 0,0100 | 0,0100 | 0,0098 | <b>0,0099</b> | 0,0002        | 0,00                  | 0,00                 |
| 29          | AES              | 0,0100  | 0,0100 | 0,0100 | 0,0100 | 0,0100 | <b>0,0100</b> | 0,0000        | 0,08                  | 0,06                 |
| 9           | AES              | 0,0090  | 0,0110 | 0,0090 | 0,0110 | 0,0110 | <b>0,0102</b> | 0,0014        | 0,23                  | 0,17                 |
| 33          | XRF              | 0,0099  | 0,0104 | 0,0102 | 0,0104 | 0,0105 | <b>0,0103</b> | 0,0003        | 0,31                  | 0,22                 |
| 13          | AES              | 0,0110  | 0,0110 | 0,0110 | 0,0090 | 0,0110 | <b>0,0106</b> | 0,0011        | 0,54                  | 0,39                 |
| 32          | AES              | 0,0112  | 0,0119 | 0,0121 | 0,0120 | 0,0118 | <b>0,0118</b> | 0,0004        | 1,46                  | 1,06                 |
| 6           | AES              | 0,0120  | 0,0120 | 0,0119 | 0,0118 | 0,0116 | <b>0,0119</b> | 0,0002        | 1,54                  | 1,11                 |
| 7           | AES              | 0,0121  | 0,0123 | 0,0126 | 0,0124 | 0,0123 | <b>0,0123</b> | 0,0002        | 1,85                  | 1,33                 |
| 4*          | AES              | 0,0210  | 0,0200 | 0,0210 |        |        | <b>0,0207</b> | 0,0014        | 8,31                  | 6,00                 |

\* - result excluded as outlier

\* - výsledek vyloučen jako odlehlý

| n  | $\bar{X} = X_{PT}$<br>[%] | S <sub>PT</sub><br>[%] | S <sub>N</sub><br>[%] | U<br>[%] |
|----|---------------------------|------------------------|-----------------------|----------|
| 16 | 0,0099                    | 0,0013                 | 0,0018                | 0,0007   |

